



ARCHIVIO ISTITUZIONALE DELLA RICERCA

Alma Mater Studiorum Università di Bologna Archivio istituzionale della ricerca

Implementing an open-access CASA software for the assessment of stallion sperm motility: Relationship with other sperm quality parameters

This is the final peer-reviewed author's accepted manuscript (postprint) of the following publication:

Published Version:

Implementing an open-access CASA software for the assessment of stallion sperm motility: Relationship with other sperm quality parameters / Giaretta, Elisa; Munerato, Mauro; Yeste, Marc; Galeati, Giovanna; Spinaci, Marcella; Tamanini, Carlo; Mari, Gaetano; Bucci, Diego. - In: ANIMAL REPRODUCTION SCIENCE. - ISSN 0378-4320. - ELETTRONICO. - 176:(2017), pp. 11-19. [10.1016/j.anireprosci.2016.11.003]

This version is available at: <https://hdl.handle.net/11585/586261> since: 2020-12-05

Published:

DOI: <http://doi.org/10.1016/j.anireprosci.2016.11.003>

Terms of use:

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

(Article begins on next page)

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>).
When citing, please refer to the published version.

This is the final peer-reviewed accepted manuscript of:

Implementing an open-access CASA software for the assessment of stallion sperm motility: Relationship with other sperm quality parameters.

Elisa Giaretta, Mauro Munerato, Marc Yeste, Giovanna Galeati, Marcella Spinaci, Carlo Tamanini, Gaetano Mari, Diego Bucci

The final published version is available online at:

<http://dx.doi.org/10.1016/j.anireprosci.2016.11.003>

Rights / License:

The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

1 **Title**

2 Implementing an open-access CASA software for the assessment of stallion sperm motility:
3 relationship with other sperm quality parameters

4

5 **Authors**

6 Elisa Giaretta¹, Mauro Munerato², Marc Yeste³, Giovanna Galeati¹, Marcella Spinaci¹,
7 Carlo Tamanini¹, Gaetano Mari^{1,4}, Diego Bucci^{1*}

8

9 **Affiliations**

10 ¹DIMEVET, Department of Veterinary Medical Sciences, Via Tolara di Sopra, 50; 40064
11 Ozzano dell'Emilia, BO, Italy

12 ²Private researcher

13 ³Biotechnology of Animal and Human Reproduction (TechnoSperm), Department of
14 Biology, Institute of Food and Agricultural Technology, University of Girona, E-17071
15 Girona, Catalonia, Spain

16 ⁴AUB INFA National Institute of Artificial Insemination, Via Gandolfi 16, 40057 Cadriano,
17 BO, Italy

18

19 ***Corresponding Author**

20 Via Tolara di Sopra 50, 40064 Ozzano dell'Emilia (BO), Italy. Email diego.bucci3@unibo.it;

21 Tel. +39 0512097912

22

23

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52

Abstract

Setting an open-access computer assisted sperm analysis (CASA) may benefit the evaluation of motility in mammalian sperm, especially when economic constraints do not allow the use of a commercial system. There have been successful attempts to develop such a device in Zebra fish sperm and the system has been used in very few studies on mammalian spermatozoa. Against this background, the present study aimed at developing an open-access CASA system for mammalian sperm using the horse as a model and based upon the Image J software previously established for Zebra fish sperm. Along with determining the sperm progressive motility and other kinetic parameters (such as amplitude of lateral head displacement), the “results” window was adjusted to simplify subsequent statistical analyses. The path window was enriched with colored sperm trajectories on the basis of the subpopulation they belong to and a number that allowed the sperm track to be associated to the sperm motility data shown in the “results” window. Data obtained from the novel plugin (named as CASA_bgm) were compared with those of the commercial CASA Hamilton-Thorn IVOS Vers.12, through Bland Altman’s plots. While the percentage of total and progressive motile sperm, VCL, VAP, VSL, LIN and STR and ALH were in agreement with those obtained with the commercial system, BCF significantly differed between the two systems probably due to their settings. Interestingly, a positive and significant correlation between the percentages of total motile sperm evaluated through CASA_bgm and those showing high mitochondrial membrane potential evaluated by JC-1 staining was found. In conclusion, CASA_bgm ImageJ plugin could be useful and reliable for stallion sperm motility analysis and it is our aim to apply this system to other mammalian species.

Keywords: CASA; stallion; sperm motility; sperm quality

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

53 1. Introduction

54

55 At present, more than 12 different computer-assisted sperm analysis (CASA)
56 systems are available for sperm motion detection in spermatology labs and in commercial
57 semen production units (Amann and Waberski, 2014). The development of a powerful
58 CASA software has made possible kinetic studies of spermatozoa and objective
59 measurements of sperm movements (Verstegen et al., 2002).

60 The evaluation of sperm motility and other kinetic parameters such as curvilinear,
61 straight line, and average path velocities, is an essential part of sperm quality examination
62 in many mammalian species. Despite the immediacy and accuracy of these softwares,
63 several investigators rely on non-automated analysis due to the high cost of commercial
64 options. CASA systems historically evolved for commercial purposes and were initially sold
65 to clinical laboratories to assess human sperm fertility (Amann and Katz, 2004). Later on,
66 CASA systems were produced for stallion sperm analysis by Hamilton-Thorne in 1986, and
67 soon after they were adapted to many species. In spite of being much widespread across
68 research laboratories, “teaching the instrument” is still needed, as reported by Amann and
69 Katz (2004).

70 The availability of an open-access, low cost CASA system could much benefit the
71 analyses of sperm motility, especially for those that, due to economic constraints, may not
72 afford the costs of a commercial device. In addition, the relevant information that a CASA
73 system provides goes beyond a more objective evaluation of the percentages of total and
74 progressive motile sperm. Indeed, some CASA systems give the individual kinetic
75 parameters for a single sperm cell and this may be used for evaluating motile sperm
76 population in differently treated samples (Abaigar et al., 1999; Flores et al., 2009, 2008;
77 Miró et al., 2005, 2009; Schmidt and Kamp, 2004; Varner, 2008). In 2007, Wilson-Leedy
78 and Ingermann developed a CASA software package that worked as a plugin to the United
79 States National Institutes of Health (NIH) Image J software (Wilson-Leedy and Ingermann,
80 2007). Successively, more than hundred scientific studies used the plugin to assess fish
81 or invertebrate sperm motility. In particular, Purchase and Earle (2012) implemented the
82 original plugin, creating a new one that permits the automation of some video processing
83 steps. Very few studies applied the system to mammalian sperm motility evaluation.
84 Elsayed et al. (2015) used the plugin to study sperm motility in bull and adapted the
85 system to their specific experimental conditions. . Boryshpolets et al. (2015) used the

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

86 original plugin to study human sperm motility in response to thermotaxis. Since this
87 plugin deposited is an open source, this allows any research laboratory to have access to
88 CASA software and to perform the motility sperm analysis.

89 The first aim of our study was to set up an Image J CASA system for mammalian
90 sperm analysis, using the horse as a model, and also including progressive motility and
91 amplitude of lateral head displacement measurements; second, we compared the results
92 obtained with our system to those of a commercial one and to the data reported in the
93 literature. Finally, we checked the correlations between motion values obtained from the
94 two CASA systems and other parameters of semen quality such as mitochondrial activity
95 and acrosome integrity.

96

97

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

98 **2. Materials and methods**

99

100 *2.1. Collection and preparation of semen*

101

102 Twenty-five ejaculates were collected from four Standardbred stallions of proven
103 fertility, individually housed at the National Institute of Artificial Insemination (University
104 of Bologna, Italy), using a Missouri artificial vagina with an inline filter (Nasco, Fort
105 Atkinson, WI, USA). Semen was diluted in Kenney's extender (Kenney et al., 1975) at a
106 semen/extender ratio of 1:3 (v:v) and sent to the laboratory within 1 h post-collection at
107 20-25°C.

108 Upon arrival, an aliquot of 2 mL of extended semen was further diluted to a final
109 concentration of 30×10^6 spermatozoa/mL, and then split into three aliquots. One was
110 evaluated with the Hamilton-Thorne CASA system Vers.12, another was evaluated with
111 the Image J software and the new CASA_bgm, and the last one was used to evaluate the
112 sperm viability with mitochondrial membrane potential and acrosome integrity.

113

114 *2.2. Video microscopy system for motility assessment*

115

116 Settings for video camera and microscope were established according to the
117 indications of Wilson-Leedy and Ingermann (2007) and a Leitz diaplan microscope (Wild
118 Leitz GmbH, D6330, Wetzlar, Germany) with a 10x plan objective with negative phase-
119 contrast was used. The microscope was equipped with a Z31A Ascon technologic heated
120 stage (Ascon technologic, PV – IT). The video camera, 3.1 megapixel CMOS USB 2.0
121 Infinity1-3 Camera (Lumenera corporation, Ottawa, ON, Canada), was coupled to the
122 microscope by a c-mount adapter and videos were registered for three seconds at a
123 resolution of 800x600 pixel and 60 frames/sec (fps). Images were recorded on a hard drive
124 using the Infinity analyzing and capture software 6.4 (Lumenera corporation) and
125 converted to avi format.

126 Prior to any observation, spermatozoa (30×10^6 sperm/mL) were loaded onto a fixed
127 height Leja Chamber SC 20-01-04-B (Leja, CIUDAD; The Netherlands). Five videos of
128 separate fields and lasting three seconds each were recorded per sperm sample.

129

130 *2.3. Installation of plugin and video adjustment and analysis*

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

131

132 The indications of Wilson-Leedy and Ingermann (2007) were followed to install the
133 plugin and to import the central second of each video. After importing, each video was
134 converted into greyscale 8-bit image and the threshold was adjusted to highlight the sperm
135 heads over the background.

136 Launching the plugin results in the initiation of a dialog box, where parameters for
137 analysis need to be indicated. In order to adapt the existing plugin to the analysis of
138 mammalian spermatozoa, the input parameters related to the bulk flow were eliminated.
139 Therefore, the dialog box generated for CASA_bgm is more simple than that of CASA and
140 the implemented input settings consisted of two VAP cut-off values that divided the sperm
141 population into slow, medium and rapid spermatozoa. The input parameters used to
142 identify and characterize the sperm motion are reported in Figure 1.

143 As shown in Figure 1a, the first two (*a* and *b*) parameters regard the minimum and
144 maximum pixel areas that the program takes into account for the analysis. The particles
145 over or below the selected area are not analyzed. The minimum track length (*c*) indicates
146 the minimum number of frames in which a particle must appear in the video in order to
147 be considered in the analysis. The maximum sperm velocity between frames (*d*) regards
148 the maximum distance a spermatozoon would be expected to travel within the time period,
149 so it is related to the sperm cells velocity.

150 The cut-off values for VSL, VAP and VCL for a spermatozoon to be considered as
151 motile are given in rows *e*, *f* and *g*. In addition, VAP cut-off values for slow and medium
152 velocity spermatozoa, which are then used to describe the sperm subpopulations based
153 upon the VAP, can be set in rows *h* and *i*. In row *l*, the user inserts the number of frames
154 acquired per second, whereas the ratio $\mu\text{m}:\text{pixels}$ of the particles analyzed should be
155 indicated in the following field (row *m*). Rows *n*, *o* and *p* are binary variables: 0 will not
156 produce the specific output, while 1 is the positive choice and will produce an output.

157 As far as the two “advanced parameters” are concerned, they were included in order
158 for the progressive motility to be determined; therefore, field *q* is the VAP cut-off and field
159 *r* is the straightness cut-off for progressive motile cells. Each analysis needs the
160 parameters to be entered correctly by the user. To automatize this procedure, Image J
161 function called Macro recorder could be used.

162

163 *2.4. Output and successive analysis*

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

164

165 Outputs obtained from CASA_bgm additional parameters were implemented to
 166 CASA plugin to match the needs of analyzing mammalian spermatozoa. The output, as the
 167 pre-existing, shows two windows: Results and Path. On the Results window, and
 168 depending on the choice made in fields n , o and p , it is possible to obtain:

169

- 170 - x and y coordinates for each spermatozoon analyzed when the number “1” is entered
 171 in field “ n ”
- 172 - motility parameters for each spermatozoon analyzed when the number “1” is
 173 selected in field “ o ” (Fig. 2)
- 174 - the mean and median values for the sperm when the number “1” is selected in field
 175 “ p ” (Fig. 2)

176

177 When typing 1 in row “ o ”, the Results window shows a list of individual sperm
 178 motion parameters, where the following values related to each spermatozoa were analyzed:
 179 VCL, VAP, VSL, LIN, STR, WOB, Beat Cross Frequency (BCF) and ALH appear in each row.
 180 Excluding ALH, algorithms for other parameter calculations are the same used in the pre-
 181 existing CASA plugin (Wilson-Leedy and Ingermann, 2007). Instead, ALH values were
 182 worked out following Mortimer (2000). Finally, the last row summarizes the total number
 183 of sperm analyzed in the selected frames.

184 By selecting the third set of parameters (row “ p ”), the output of Results shows
 185 average (Avg) and median (Median) values for the populations of sperm examined, with the
 186 respective standard deviations (Sigma). Additionally, the same output shows the numbers
 187 of total (Total Sperm), total motile (TM), progressive motile (PM), slow, medium and rapid
 188 spermatozoa analyzed. If multiple analyses are performed, the results of each analysis are
 189 added to new rows below and are depicted in the Results window. Moreover, the plugin
 190 also produces an output window called *Path* (Fig. 3), that is an image showing the paths
 191 of each single spermatozoon. In CASA_bgm, black marks identify non-motile sperm, whilst
 192 paths of motile sperm are traced with different colors indicating different velocities, so that
 193 red, yellow and green colors are utilized for rapid, medium and slow sperm, respectively.
 194 This classification is made on the basis of VAP. In addition, each path of motile sperm is
 195 tagged with an ordinal number that corresponds to the order through which spermatozoa
 196 are listed in the Results windows.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

197

198

199 *2.5. Image J settings (Macro Horse)*

200

201 We set the parameters for performing the motility analysis with horse spermatozoa
202 in accordance to the Standard Operating Procedure of Italian Experimental Institute
203 “Lazzaro Spallanzani” (Law D.M. 403/2000). The same values of VAP and STR for PM
204 evaluation were used for the analyses with Hamilton CASA system.

205 The parameters chosen for this purpose are shown in Figure 1.

206

207 *2.6. Motility evaluation using Hamilton CASA system*

208

209 Motility was measured using a Hamilton Thorne, IVOS Ver. 12. Sperm cells were
210 evaluated for each sample diluted to 30×10^6 sperm/mL using a fixed-height Leja Chamber
211 SC 20-01-04-B (Leja, The Netherlands). The assessed sperm motility were: proportions of
212 total motile (TM) and progressive motile (PM) spermatozoa, curvilinear velocity (VCL, $\mu\text{m}\cdot\text{s}^{-1}$)
213 mean velocity (VAP, $\mu\text{m}\cdot\text{s}^{-1}$), straight-line velocity (VSL, $\mu\text{m}\cdot\text{s}^{-1}$), straightness (STR, %),
214 linearity (LIN, %), beat cross frequency (BCF, Hz), and amplitude of lateral head
215 displacement (ALH, μm). The settings were as follows, frames per second: 60; number of
216 frames: 45; threshold path velocity: $15 \mu\text{m}\cdot\text{s}^{-1}$; and straightness threshold: 75%.

217

218 *2.7. Sperm mitochondrial activity and viability and acrosome integrity*

219 Unless otherwise stated, all chemicals were purchased from Sigma–Aldrich (Milan,
220 Italy).

221

222 *2.7.1. Evaluation of mitochondrial activity and viability*

223 For each sample, an aliquot (25 μL) of semen (30×10^6 spermatozoa/mL) was
224 incubated with 2 μL of a 300 μM propidium iodide (PI) stock solution, 2 μL of a 10 μM
225 SYBR green-14 stock solution, both obtained from the live/dead sperm viability kit
226 (Molecular Probes, Inc.) and 2 μL of a 150 μM JC-1 solution for 20 min at 37°C in the
227 dark. Ten μL of the sperm suspension were then placed on a slide and at least 200
228 spermatozoa per sample were scored using a Nikon Eclipse E 600 epifluorescence
229 microscope (Nikon Europe BV, Badhoevedop, The Netherlands). Spermatozoa stained

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

230 with SYBR-14 but not with PI were considered as viable (SYBR-14⁺/PI⁻), whereas SYBR-
231 14⁺/PI⁺ and SYBR-14⁻/PI⁺ spermatozoa were considered as non-viable. JC-1 monomers
232 emit green fluorescence in mitochondria with low membrane potential (JC-1⁻) and form
233 aggregates in mitochondria with high membrane potential (JC-1⁺), then emitting a bright
234 red-orange fluorescence. Therefore, those viable sperm showing orange-red fluorescence
235 in the mid piece (JC-1⁺) were considered as viable sperm with high mitochondrial
236 membrane potential (SYBR-14⁺/PI⁻/JC-1⁺).

237

238 *2.7.2. Evaluation of acrosome integrity*

239 The integrity of the acrosome was evaluated using FITC-conjugated agglutinin
240 derived from *Pisum sativum* (FITC-PSA) that specifically binds to α -mannoside sugar
241 residues found within the acrosomal contents. Briefly, spermatozoa were washed twice
242 with PBS and subsequently fixed and permeabilized with 95% ethanol at -20°C for 30 min.
243 Sperm were placed onto microscope slides, air-dried, and incubated with FITC-PSA (0.1
244 mg/mL PSA-FITC) for 15 min at room temperature in the dark. Samples were finally
245 examined under the aforesaid microscope, and 200 cells were counted. Acrosomes were
246 considered as intact when stained with FITC-PSA, and damaged when presenting total or
247 partial loss of FITC-PSA- fluorescence.

248

249 *2.8. Statistical analyses*

250 Data were analyzed with a statistical package (IBM SPSS for Windows Ver 21.0; IBM
251 Corp., Chicago, IL, USA) and are expressed as mean \pm standard deviation. After
252 determining the normality and homogeneity of variances through Shapiro-Wilk and Levene
253 tests, a t-test comparing the two CASA devices was conducted. Data were transformed
254 through \sqrt{x} or $\arcsin \sqrt{x}$ when required. The agreement between the two systems' results
255 was studied by Bland Altman's plots. Correlations between kinetic parameters and sperm
256 viability, mitochondrial activity and acrosome integrity were determined through Pearson
257 correlation. In all cases, the level of significance was at least at $P \leq 0.05$.

258

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

259 **3. Results**

260

261 Motility parameters obtained from CASA_bgm plugin and Hamilton-Thorne IVOS
262 are shown in Table 1. Total and progressive motility values were similar, with no significant
263 differences between paired samples.

264 The agreement between the two systems' measurements was assessed by Bland
265 Altman's Plot (see Supplementary file 1). The different parameters showed a good
266 agreement, in particular TM, PM, VAP, VSL, STR, LIN. VCL, BCF and ALH showed good
267 agreement with some data outside the ± 2 SD.

268 Tables 2 and 3 show the correlation between sperm motility parameters, evaluated
269 through the two CASA systems (CASA_bgm and Hamilton CASA respectively), and the
270 percentages of viable sperm cells with active mitochondria (SYBR-14⁺/PI⁻/JC-1⁺) and
271 sperm with intact acrosomes (PSA⁺).

272 Results from CASA_bgm showed a significant positive correlation with the
273 percentage of motile sperm (total motility) and the percentage of SYBR-14⁺/PI⁻/JC-1⁺
274 sperm ($P < 0.001$). Moreover, motility variables such as VAP, VSL and WOB evaluated
275 through CASA_bgm showed a significant negative correlation with the percentage of sperm
276 exhibiting an intact acrosome ($P < 0.05$). Finally, a significant positive correlation between
277 BCF evaluated by CASA_bgm and sperm with intact acrosomes was observed ($P < 0.05$).

278 With regard to the motility parameters obtained through Hamilton CASA analysis,
279 only a significant negative relationship between ALH and sperm with intact acrosome was
280 observed ($P < 0.01$).

281

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

282 4. Discussion

283

284 The present study aimed at setting an open-access CASA system for evaluating the
285 motility of mammalian sperm from adapting the system developed by Wilson-Leedy and
286 Ingermann , (2007) for fish sperm. In effect, the original ImageJ-plugin created by these
287 Authors was intended to fish sperm and, consequently, requires some adaptation and
288 implementation to fit the request of a standard mammalian sperm analysis. Therefore, the
289 first objective was to modify the previously mentioned plugin, adding the progressive
290 motility and amplitude of lateral head displacement, that were absent in the original
291 version. For this purpose, two new fields were added to the input window and an algorithm
292 was created *ex novo*. Moreover, we included three additional fields in the input window in
293 order to classify as “slow”, “medium” and “rapid” spermatozoa, as other systems, like the
294 Hamilton-Thorne IVOS, do.

295 After adding or completing the input setup, we also introduced some modifications
296 in the output window. Briefly, we included the progressively motile sperm count (PM) and
297 amplitude of lateral head displacement measure (ALH) in the outputs, as well as the
298 number of total motile sperm and the total count of sperm analyzed. This allows a better
299 and faster use of these data for further statistical analyses. Regarding the “Paths” window,
300 our output allows to distinguish through the track color between static (black paths), slow
301 (green paths), medium (yellow paths) and fast (red paths) sperm. This classification
302 originates from the different cut-off VAP values, which are set in the input window and
303 may be modified and adapted to the peculiarities of other mammalian species. In addition,
304 each sperm track is associated with a number, which allows the user to identify quickly (if
305 sperm concentration is not too high) the path of a given spermatozoon and to associate it
306 with the single data obtained in the results window. Thus, each number corresponds to a
307 specific line in the results window (e.g. number 1 correspond to the first row, etc.).

308 We analyzed 25 samples from four stallions with both Hamilton-Thorne IVOS and
309 CASA_bgm Image J plugin. To avoid any technical differences, we used the same sperm
310 concentration for both instruments, as recommended by Holt and colleagues (Holt et al.,
311 1996, 1994). Leja chambers were also used, as it is well known that different supports
312 yield different results on the motility parameters (Hoogewijs et al., 2012). Finally, our
313 settings for determining the sperm motion took into account previous studies. Indeed, and
314 as reported by (Holt et al., 1996), there have been several approaches to detect properly

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

315 the true movements of sperm cells, and to distinguish motile from non-motile spermatozoa.
316 In this regard, it has been reported that VAP values around $20 \mu\text{m}\cdot\text{s}^{-1}$ or less could be due
317 to spurious movements of non-viable sperm.

318 It is worth noting that our results on TM, PM, VCL, VAP, VSL, STR and LIN obtained
319 with CASA_bgm are consistent with those obtained by the Hamilton-Thorne CASA. It
320 should be pointed out that data from our instrument and the commercial one are
321 numerically different, but the excursion of measurements between the two systems is not
322 significant. Our coefficients of variation are also in agreement with data reported by other
323 Authors (Holt et al., 1994), who found values exceeding 20%. In that work, CV for total
324 motility, VCL, VAP, LIN and ALH were 24%, 19%, 44%, 22.5% and 39%, respectively. The
325 higher degree of variation of that work is possibly due to the comparison between
326 numerous systems (five CASA). In the present study, although Hamilton Thorne CASA
327 showed lower CV than CASA_bgm, the extent of these differences was not as high as that
328 reported by other Authors (Holt et al., 1994). Moreover, BCF, was quite different between
329 the two systems. This could be due to the difference in the algorithms between software.
330 Indeed, various CASA systems, which generally utilize proprietary software, use different
331 algorithms to determine the same measures. Therefore, in the absence of a “gold standard”
332 with reference value, internal validation is required, which is setting-, system-, and
333 species- specific (Amann and Waberski, 2014).

334 Besides, a new parameter ALH, not originally present in the Image J CASA, was set
335 on the basis of the algorithm proposed by Mortimer (2000). In this context, it is worth
336 noting that Holt et al. (1994) reported that caution is needed when comparing results
337 between CASA systems, particularly with regard to ALH and VAP. Not only do our data
338 support this idea, but also indicate that such assertion could be extended to the other
339 kinetic parameters. In addition, sperm preparation, previous incubation periods, qualities
340 of optics, camera and imaging are amongst the factors responsible for the differences
341 between CASA devices. Therefore, a direct comparison between such devices is not possible
342 (Holt et al., 1996). Apart from this, one should note that other researchers have also
343 pointed out additional critical steps in semen motility analysis, ranging from sample
344 preparation (Contri et al., 2010) to the support used (Hoogewijs et al., 2012).

345 The original plugin was already tested with fish sperm in comparison with two other
346 systems (Boryshpolets et al., 2013). In that study, Image J plugin was shown to be in
347 accordance with the other two examined systems, but for determined conditions (different

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

348 frame rate) and fish species, VCL from Image J and CRISMAS CASA systems were in
349 accordance, while the Hobson Sperm Tracker was not.

350 Since a reliable method to evaluate sperm motility should give a global picture of
351 sperm quality and should be in agreement with other sperm parameters, such membrane
352 integrity, the second part of the work was intended to correlate the motility values obtained
353 from the two CASA systems with sperm mitochondrial activity and acrosome integrity.
354 Interestingly, we observed that the motion values obtained by CASA_bgm were better
355 correlated with the other sperm quality parameters than those obtained through the
356 commercial CASA. Indeed, a significant positive correlation between TM and the
357 percentage of SYBR-14⁺/PI-/JC-1⁺ positive sperm was observed, kinetic parameters such
358 as VAP, VSL and WOB showed a significant negative correlation with the percentage of
359 sperm exhibiting an intact acrosome. The correlation between TM and viability and
360 mitochondrial activity has been previously demonstrated (Bucci et al., 2016; Plaza Dávila
361 et al., 2015). The significant and positive correlation between all these parameters
362 corroborates the reliability of CASA_bgm. Moreover the relationship between the single
363 kinetic sperm characteristics and its functional status, in terms of viability, mitochondrial
364 activity and acrosome integrity, could be interesting for further investigations, since they
365 could improve the predictive accuracy of the true sperm's fertilizing potential ((Jung et al.,
366 2015; Nagy et al., 2015; Oliveira et al., 2013; Santolaria et al., 2015). In addition, the
367 motion values of individual spermatozoon analyzed, which can be recorded by CASA_bgm,
368 could be useful to study sperm subpopulations, after various techniques for processing
369 semen, such as cryopreservation, capacitation or hyperactivation (Henning et al., 2014;
370 Martínez-Pastor et al., 2011). In fact, mounting evidence indicates that the distribution of
371 spermatozoa in different subpopulations based on motion features may have functional
372 relevance and can be useful to study sperm biology (Amann and Waberski, 2014).

373 Finally, and as for the possibility of using CASA_bgm for other mammalian species,
374 it is possible to establish specific settings for each species analyzed and to easily modify
375 these parameters in the input. Two studies applied so far the original CASA plugin to
376 mammalian species (Boryshpolets et al., 2015; Elsayed et al., 2015): the first one analyzed
377 human sperm motility parameters (only VCL, VAP, VSL, LIN and WOB) by the enhanced
378 CASA version (Purchase and Earle, 2012). Those Authors studied the thermotactic
379 behavior of spermatozoa subjected to different temperature (31°C then 37°C and again
380 31°C) and obtained interesting results on sperm parameters changes. The second study

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

381 developed a new CASA system for the analysis of bull spermatozoa under very particular
382 experimental conditions: in fact, those Authors implemented the original plugin to study
383 bull spermatozoa in different microfluidic environments. These two studies demonstrate
384 that the plugin is reliable and could also be used properly for mammalian sperm. Anyway,
385 Boryshpolets et al. (2015) did not improve the original plugin, while Elsayed et al. (2015)
386 did improve it, with very new peculiar parameters (orientation, proximity to wall,
387 swimVAP). In the present work, we added progressive motility (PM) and amplitude of lateral
388 head displacement (ALH), two parameters that are important for all sperm analyses and
389 also for detecting or defining hyperactivation (Cremades et al., 2005; Schmidt and Kamp,
390 2004). Furthermore, being this software an open source, any investigator may freely
391 implement or modify (as we and others already did) the plugin and create a more specific
392 or versatile system, according to his/her needs; this could then be made available to the
393 whole scientific community, which would benefit from that tool.

394 In conclusion, the present study demonstrates the possibility of implementing an
395 open-access CASA for evaluating stallion sperm motility and to easily adapt this
396 background to other mammalian species. Whilst no “gold standard” is available to assert
397 which system is the most suitable, the high and significant correlation of those sperm
398 kinetic parameters evaluated through CASA_bgm with other sperm quality parameters,
399 including membrane integrity and mitochondrial activity, demonstrates the reliability of
400 this tool. This open source system could benefit those researchers that cannot afford the
401 purchase of a commercial CASA system.

402

403 The plugin is provided as an e-component of the present article (see e-component.
404 BGM_java)

405

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

406 **References**

407

408 Abaigar, T., Holt, W. V, Harrison, R. a, del Barrio, G., 1999. Sperm subpopulations in
 409 boar (*Sus scrofa*) and gazelle (*Gazella dama mhorr*) semen as revealed by pattern
 410 analysis of computer-assisted motility assessments. *Biol. Reprod.* 60, 32–41.
 411 doi:10.1095/biolreprod60.1.32

412 Amann, R.P., Katz, D.F., 2004. Andrology Lab Corner*: Reflections on CASA After 25
 413 Years. *J Androl* 25, 317–325. doi:10.1002/j.1939-4640.2004.tb02793.x

414 Amann, R.P., Waberski, D., 2014. Computer-assisted sperm analysis (CASA):
 415 Capabilities and potential developments. *Theriogenology* 81, 5–17.
 416 doi:10.1016/j.theriogenology.2013.09.004

417 Boryshpolets, S., Kowalski, R.K., Dietrich, G.J., Dzyuba, B., Ciereszko, A., 2013.
 418 Different computer-assisted sperm analysis (CASA) systems highly influence sperm
 419 motility parameters. *Theriogenology* 80, 758–765.
 420 doi:10.1016/j.theriogenology.2013.06.019

421 Boryshpolets, S., P??rez-Cerezales, S., Eisenbach, M., 2015. Behavioral mechanism of
 422 human sperm in thermotaxis: A role for hyperactivation. *Hum. Reprod.* 30, 884–892.
 423 doi:10.1093/humrep/dev002

424 Bucci, D., Giaretta, E., Spinaci, M., Rizzato, G., Isani, G., Mislei, B., Mari, G., Tamanini,
 425 C., Galeati, G., 2016. Characterization of alkaline phosphatase activity in seminal
 426 plasma and in fresh and frozen-thawed stallion spermatozoa. *Theriogenology* 85,
 427 288–295. doi:10.1016/j.theriogenology.2015.09.007

428 Contri, A., Valorz, C., Faustini, M., Wegher, L., Carluccio, A., 2010. Effect of semen
 429 preparation on casa motility results in cryopreserved bull spermatozoa.
 430 *Theriogenology* 74, 424–435. doi:10.1016/j.theriogenology.2010.02.025

431 Cremades, T., Roca, J., Rodriguez-Martinez, H., Abaigar, T., Vazquez, J.M., Martinez, E.
 432 a, 2005. Kinematic changes during the cryopreservation of boar spermatozoa. *J.*
 433 *Androl.* 26, 610–8. doi:10.2164/jandrol.05028

434 Elsayed, M., El-Sherry, T.M., Abdelgawad, M., 2015. Development of computer-assisted
 435 sperm analysis plugin for analyzing sperm motion in microfluidic environments

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

- 436 using Image-J. *Theriogenology* 84, 1367–1377.
437 doi:10.1016/j.theriogenology.2015.07.021
- 438 Flores, E., Fernández-Novell, J.M., Peña, A., Rodríguez-Gil, J.E., 2009. The degree of
439 resistance to freezing-thawing is related to specific changes in the structures of
440 motile sperm subpopulations and mitochondrial activity in boar spermatozoa.
441 *Theriogenology* 72, 784–797. doi:10.1016/j.theriogenology.2009.05.013
- 442 Flores, E., Taberner, E., Rivera, M., Peña, A., 2008. Effects of freezing/thawing on motile
443 sperm subpopulations of boar and donkey ejaculates. *Theriogenology* 70, 936–945.
444 doi:10.1016/j.theriogenology.2008.05.056
- 445 Henning, H., Petrunkina, A.M., Harrison, R.A.P., Waberski, D., 2014. Cluster analysis
446 reveals a binary effect of storage on boar sperm motility function, in: *Reproduction,*
447 *Fertility and Development*. pp. 623–632. doi:10.1071/RD13113
- 448 Holt, C., Holt, W. V, Moore, H., 1996. Choice of Operating Conditions to Minimize Sperm
449 Subpopulation Sampling Bias in the Assessment of Boar Semen by Computer-
450 Assisted Semen Analysis. *J Androl* 17, 587–596.
- 451 Holt, W., Watson, P., Curry, M., Holt, C., 1994. Reproducibility of computer-aided semen
452 analysis: comparison of five different systems used in a practical workshop. *Fertil.*
453 *Steril.* 62, 1277–1282.
- 454 Hoogewijs, M.K., De Vlieghe, S.P., Govaere, J.L., De Schauwer, C., De Kruif, A., Van
455 Soom, A., 2012. Influence of counting chamber type on CASA outcomes of equine
456 semen analysis. *Equine Vet. J.* 44, 542–549. doi:10.1111/j.2042-
457 3306.2011.00523.x
- 458 Jung, M., Rüdiger, K., Schulze, M., 2015. In Vitro Measures for Assessing Boar Semen
459 Fertility. *Reprod. Domest. Anim.* 50, 20–24. doi:10.1111/rda.12533
- 460 Martínez-Pastor, F., Tizado, E.J., Garde, J.J., Anel, L., de Paz, P., 2011. Statistical
461 Series: Opportunities and challenges of sperm motility subpopulation analysis.
462 *Theriogenology*. doi:10.1016/j.theriogenology.2010.11.034
- 463 Miró, J., Lobo, V., Quintero-Moreno, a, Medrano, a, Peña, a, Rigau, T., 2005. Sperm
464 motility patterns and metabolism in Catalanian donkey semen. *Theriogenology* 63,
465 1706–16. doi:10.1016/j.theriogenology.2004.07.022

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

- 466 Mirò, J., Taberner, E., Rivera, M., Pe??a, A., Medrano, A., Rigau, T., Pe??alba, A., 2009.
 467 Effects of dilution and centrifugation on the survival of spermatozoa and the
 468 structure of motile sperm cell subpopulations in refrigerated Catalanian donkey
 469 semen. *Theriogenology* 72, 1017–1022. doi:10.1016/j.theriogenology.2009.06.012
- 470 Mortimer, S.T., 2000. CASA--practical aspects. *J. Androl.* 21, 515–524.
 471 doi:10.1002/j.1939-4640.2000.tb02116.x
- 472 Nagy, Á., Polichronopoulos, T., Gáspárdy, A., Solti, L., Cseh, S., 2015. Correlation
 473 between bull fertility and sperm cell velocity parameters generated by computer-
 474 assisted semen analysis. *Acta Vet. Hung.* 63, 370–81. doi:10.1556/004.2015.035
- 475 Oliveira, L.Z., Arruda, R.P. de, Andrade, A.F.C. de, Celeghini, E.C.C., Reeb, P.D., Martins,
 476 J.P.N., Santos, R.M. dos, Beletti, M.E., Peres, R.F.G., Monteiro, F.M., Hossepian de
 477 Lima, V.F.M., 2013. Assessment of in vitro sperm characteristics and their
 478 importance in the prediction of conception rate in a bovine timed-AI program. *Anim.*
 479 *Reprod. Sci.* 137, 145–155. doi:10.1016/j.anireprosci.2013.01.010
- 480 Plaza Dávila, M., Bucci, D., Galeati, G., Peña, F., Mari, G., Giaretta, E., Tamanini, C.,
 481 Spinaci, M., 2015. Epigallocatechin-3-Gallate (EGCG) Reduces Rotenone Effect on
 482 Stallion Sperm-Zona Pellucida Heterologous Binding. *Reprod. Domest. Anim.* 50,
 483 1011–1016. doi:10.1111/rda.12628
- 484 Purchase, C.F., Earle, P.T., 2012. Modifications to the imagej computer assisted sperm
 485 analysis plugin greatly improve efficiency and fundamentally alter the scope of
 486 attainable data. *J. Appl. Ichthyol.* 28, 1013–1016. doi:10.1111/jai.12070
- 487 Santolaria, P., Vicente-Fiel, S., Palacín, I., Fantova, E., Blasco, M.E., Silvestre, M.A.,
 488 Yániz, J.L., 2015. Predictive capacity of sperm quality parameters and sperm
 489 subpopulations on field fertility after artificial insemination in sheep. *Anim. Reprod.*
 490 *Sci.* 163, 82–88. doi:10.1016/j.anireprosci.2015.10.001
- 491 Schmidt, H., Kamp, G., 2004. Induced hyperactivity in boar spermatozoa and its
 492 evaluation by computer-assisted sperm analysis. *Reproduction* 128, 171–179.
 493 doi:10.1530/rep.1.00153
- 494 Varner, D.D., 2008. Developments in stallion semen evaluation. *Theriogenology* 70, 448–
 495 462. doi:10.1016/j.theriogenology.2008.04.023

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

- 496 Verstegen, J., Iguer-Ouada, M., Onclin, K., 2002. Computer assisted semen analyzers in
497 andrology research and veterinary practice, in: *Theriogenology*. pp. 149–179.
498 doi:10.1016/S0093-691X(01)00664-1
- 499 Wilson-Leedy, J.G., Ingermann, R.L., 2007. Development of a novel CASA system based
500 on open source software for characterization of zebrafish sperm motility parameters.
501 *Theriogenology* 67, 661–672. doi:10.1016/j.theriogenology.2006.10.003
- 502
- 503 D.M. 403/2000 e 27.12.1994. Controllo Ufficiale del Seme. POS - Protocollo Operativo
504 Standard Anno 2013. Istituto Sperimentale Italiano Lazzaro Spallanzani.
505

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

506 Table 1. Motility parameters from CASA_bgm and Hamilton-Thorne IVOS

507

	CASA_bgm	% CV	IVOS	% CV	Paired <i>t</i> -test p value	% Total CV
% TM	75.27±10.80	18.22	78.64±11.43	14.23	=0.05	16.64
% PM	37.04±11.21	30.36	37.96±9.33	24.97	>0.05	27.62
VCL	203.24±33.67	16.50	190.78±19.43	9.61	>0.05	13.69
VAP	110.98±26.81	22.88	101.20±13.54	13.30	>0.05	19.29
VSL	75.02±15.20	18.89	71.49±11.52	17.35	>0.05	18.06
LIN	38.20±5.70	14.49	38.12±3.94	11.78	>0.05	13.12
STR	69.25±7.13	9.51	69.44±5.12	7.95	>0.05	8.69
WOB	54.21±6.94	12.32	NA	NA	NA	12.32
BCF	28.19±2.39	9.11	40.78±2.40	6.18	<0.01	20.69
ALH	8.10±1.49	17.78	7.64±0.51	7.45	>0.05	14.01

508

509 Abbreviations: TM – total sperm motility; PM – Progressive sperm motility; VAP – average
510 path velocity; VSL – straight line velocity; VCL – curvilinear velocity; ALH – amplitude of
511 lateral head displacement; BCF– beat cross frequency; STR – straightness of track; LIN –
512 linearity of track; WOB – wobble. CV – coefficient of variation. Data are reported as mean
513 ± SD.

514

515

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

516 Table 2. Correlation between CASA_bgm parameters and percentage of sperm with
 517 intact acrosome and percentage of viable sperm with active mitochondria. *P<0.05
 518 **P<0.01

519

	% Sperm with an intact acrosome	% SYBR-14 ⁺ /PI ⁻ /JC-1 ⁺ -sperm
TM	0.32	0.47**
PM	0.33	0.17
VCL	-0.24	0.28
VAP	-0.39*	0.21
VSL	-0.45*	0.17
LIN	-0.25	-0.17
STR	0.08	-0.10
WOB	-0.41*	-0.05
BCF	0.38*	0.11
ALH	-0.31	0.25

520

521 Abbreviations: TM – total sperm motility; PM – Progressive sperm motility; VAP – average
 522 path velocity; VSL– straight line velocity; VCL – curvilinear velocity; ALH – amplitude of
 523 lateral head displacement; BCF – beat cross frequency; STR – straightness of track; LIN –
 524 linearity of track; WOB - wobble.

525

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

526 Table 3. Correlation between IVOS Hamilton-Thorne CASA parameters and percentage
 527 of cells with intact acrosome and percentage of viable sperm with active mitochondria.
 528 *P<0.05.

529

	% Sperm with an intact acrosome	% SYBR-14+/PI-/JC-1+ -sperm
TM	0.13	0.26
PM	-0.07	0.33
VCL	-0.04	-0.07
VAP	-0.10	-0.13
VSL	-0.25	-0.04
LIN	-0.16	0.02
STR	-0.22	0.17
WOB	-0.14	-0.19
BCF	0.32	-0.23
ALH	-0.36*	0.20

530

531 Abbreviations: TM – total sperm motility; PM – Progressive sperm motility; VAP – average
 532 path velocity; VSL– straight line velocity; VCL – curvilinear velocity; ALH – amplitude of
 533 lateral head displacement; BCF – beat cross frequency; STR – straightness of track; LIN –
 534 linearity of track; WOB - wobble.

535

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

536 Figure 1.

537

Figure 1 shows two versions of the Sperm Tracker input dialog box. The left version (a) is the original dialog box, and the right version (b) is the modified version for mammalian sperm analysis. The parameters and their values are as follows:

Parameter	Value
a, Minimum sperm area (pixels ²):	15
b, Maximum sperm area (pixels ²):	150
c, Minimum track length (frames):	30
d, Maximum sperm velocity between frames (pixels):	40
e, Minimum VSL for motile (um/s):	10
f, Minimum VAP for motile (um/s):	15
g, Minimum VCL for motile (um/s):	25
h, Maximum VAP for SLOW (um/s):	30
i, Maximum VAP for MEDIUM (um/s):	80
l, Frame Rate (frames per second):	60
m, Microns per 1000 pixels:	500
n, Print xy co-ordinates for all tracked sperm?(1 Yes, 0 No)	0
o, Print motion characteristics for all motile sperm?(1 Yes, 0 No)	1
p, Print mean and median values for motion characteristics?(1 Yes, 0 No)	1
----- ADVANCED PARAMETERS -----	
q, Minimum VAP for PM	15
r, Minimum STR for PM (%)	75

Parameter	Value
a, Minimum sperm size (pixels):	0
b, Maximum sperm size (pixels):	40.0000
c, Minimum track length (frames):	97.0000
d, Maximum sperm velocity between frames (pixels):	8.00000
e, Minimum VSL for motile (um/s):	3.000
f, Minimum VAP for motile (um/s):	20.0000
g, Minimum VCL for motile (um/s):	25.0000
h, Low VAP speed (um/s):	5.00000
i, Maximum percentage of path with zero VAP:	1.0
j, Maximum percentage of path with low VAP:	25.0000
k, Low VAP speed 2 (um/s):	25.0000
l, Low VCL speed (um/s):	35.0000
m, High WOB (percent VAP/VCL):	80.0000
n, High LIN (percent VSL/VAP):	80.0000
o, High WOB two (percent VAP/VCL):	50.0000
p, High LIN two (percent VSL/VAP):	60.0000
q, Frame Rate (frames per second):	97.0000
r, Microns per 1000 pixels:	1075.00
s, Print xy co-ordinates for all tracked sperm?	0
t, Print motion characteristics for all motile sperm?	0
u, Print median values for motion characteristics?	0

538

539 Figure 1. CASA_bgm (a) and CASA_ (b) sperm tracker input dialog box. Some fields from
 540 the original input dialog box have been removed as not necessary for mammalian sperm
 541 analysis.

542

543

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

544 Figure 2

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

Parameters for motile sperm									
VCL	VAP	VSL	LIN	STR	WOB	BeatCross	ALH		
208.4422	117.5997	92.12508	0.441969	0.783379	0.564184	22.69231	6.781614		
57.10527	33.98052	33.06013	0.578933	0.972914	0.595051	33.12281	2.076376		
129.6436	50.9638	40.01078	0.308621	0.785082	0.393107	31.05263	5.116851		
144.441	70.79696	41.66586	0.288463	0.588526	0.490145	32.18182	5.977822		
244.0964	100.948	21.53316	0.088216	0.213309	0.413558	31.05263	9.370712		
180.4653	73.34014	68.32744	0.378618	0.931651	0.406395	30.51724	5.03472		
204.4206	92.29341	71.11768	0.347899	0.770561	0.451488	31.95833	8.313763		
187.8413	92.70441	72.69722	0.387014	0.784183	0.493525	21.73684	6.442191		
102.7384	68.11353	59.32798	0.577467	0.871016	0.662981	33.39623	3.969582		
199.5729	90.0397	33.60023	0.168361	0.373171	0.451162	36.22807	7.658349		
241.8574	106.7313	41.69513	0.172396	0.390655	0.441299	33.71429	9.16523		
208.7	86.18127	49.3397	0.236414	0.572511	0.412943	37.84906	7.227401		
76.0532	19.15179	15.73174	0.206852	0.821424	0.251821	25.87719	1.602928		
140.6687	66.61184	61.41458	0.43659	0.921977	0.473537	33.1875	4.324525		
121.0462	65.35769	62.766	0.518529	0.960346	0.53994	28.9434	4.557494		
54.04993	18.49949	17.39703	0.32187	0.940406	0.342267	35.19298	2.233654		
115.7715	46.49909	40.86501	0.35298	0.878835	0.401645	26.71698	3.260101		
108.198	43.05379	33.07	0.305644	0.768109	0.397917	31.60714	4.58126		
180.2396	77.94228	72.54892	0.402514	0.930803	0.432437	28.48276	6.111791		
100.9077	29.959	24.90571	0.246817	0.831327	0.296895	28.98246	2.371706		
132.0983	73.93782	68.84734	0.521182	0.931152	0.559718	26.22222	4.748324		
203.0996	90.36935	37.69428	0.185595	0.417113	0.444951	32.08772	6.62122		
91.42439	66.02258	60.7103	0.664049	0.919538	0.722155	30.01754	4.684298		
81.10976	30.64762	23.28496	0.28708	0.759764	0.377854	30.55357	3.196392		
171.3814	67.98292	20.4941	0.119582	0.30146	0.396676	23.17857	5.500337		
194.5852	89.10887	80.53256	0.413868	0.903755	0.457943	28.60606	7.859629		
92.89756	63.31046	58.71605	0.632052	0.92743	0.681508	28.98246	3.358674		
79.45986	32.02757	29.26935	0.368354	0.91388	0.403066	34.15789	3.14254		
98.73236	64.23033	36.09186	0.365553	0.561913	0.65055	23.80702	4.135894		
192.1678	104.9203	74.44733	0.387408	0.709561	0.545983	25.87719	7.032392		
109.3685	52.77604	39.45234	0.360729	0.747543	0.482552	32.08772	4.843184		
72.93187	35.76814	33.78304	0.463214	0.944501	0.490432	28.98246	3.288517		
88.70194	42.0184	18.73911	0.211259	0.445974	0.473703	30.01754	3.674224		
71.0462	35.08382	29.83453	0.419931	0.850379	0.493817	38.29824	2.85478		
190.4572	96.78941	85.78745	0.450429	0.886331	0.508195	31.23529	7.854505		
195.9439	109.1582	96.40215	0.491988	0.883142	0.557089	31.46667	9.582038		
200.0686	100.7108	54.26265	0.27122	0.538797	0.503381	34.22	7.64082		
223.7871	82.24772	23.39241	0.10453	0.284414	0.367527	22.87755	8.010928		
140.1676	84.55843	78.46845	0.559819	0.927979	0.603267	30.15556	5.648967		
174.6872	68.16888	56.45772	0.323193	0.828204	0.390234	27.53333	5.39762		
151.3767	39.70294	29.18845	0.19282	0.735171	0.262279	28.48276	2.023471		
78.01864	61.79254	58.24905	0.746604	0.942655	0.792023	29.5	2.284161		
55.20258	22.50139	20.29848	0.367709	0.902099	0.407615	17.7	1.631619		
120.6371	60.33001	56.47726	0.468158	0.936139	0.500095	22.37931	5.266281		
145.6646	97.53716	88.55895	0.607965	0.907951	0.669601	21.07143	6.907838		
128.6104	49.32986	40.31792	0.313489	0.817313	0.38356	26.22222	4.369081		
TotalSperm	68								
TM	PM	AvgVCL	AvgVAP	AvgVSL	AvgLIN	AvgSTR	AvgWOB	AvgBeats	AvgALH
46	32	141.0845	66.77824	48.97734	0.370955	0.761181	0.473321	29.35246	5.16817
SLOW	MEDIUM	RAPID							
4	26	16							
MedianVCL	MedianVAP	MedianVSL	MedianLIN	MedianSTR	MedianWC	MedianBea	MedianALH		
136.133	67.29738	41.6805	0.366631	0.829765	0.46574	30.01754	4.938952		
SigmaVCL	SigmaVAP	SigmaVSL	SigmaLIN	SigmaSTR	SigmaWOB	SigmaBeats	SigmaALH		
54.43197	26.79796	22.59057	0.153401	0.209589	0.116159	4.522693	2.198211		
#####	---	Color	LEGEND	---	#####				
RED:	RAPID								
ORANGE:	MEDIUM								

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

BLACK: NOT CLASSIFIED

When citing, please refer to the published version.

546

547 *Figure 2.* Output window produced by the plugin when the choice “1” is set at “o” and ”p”
548 fields. In case “o” field is set to “0”, motility characteristics from single cells are not
549 displayed; when “p” field is set to “0”, median, mean values and standard deviations of the
550 analyzed video are not displayed.

551


552

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

553

554 Figure 3.

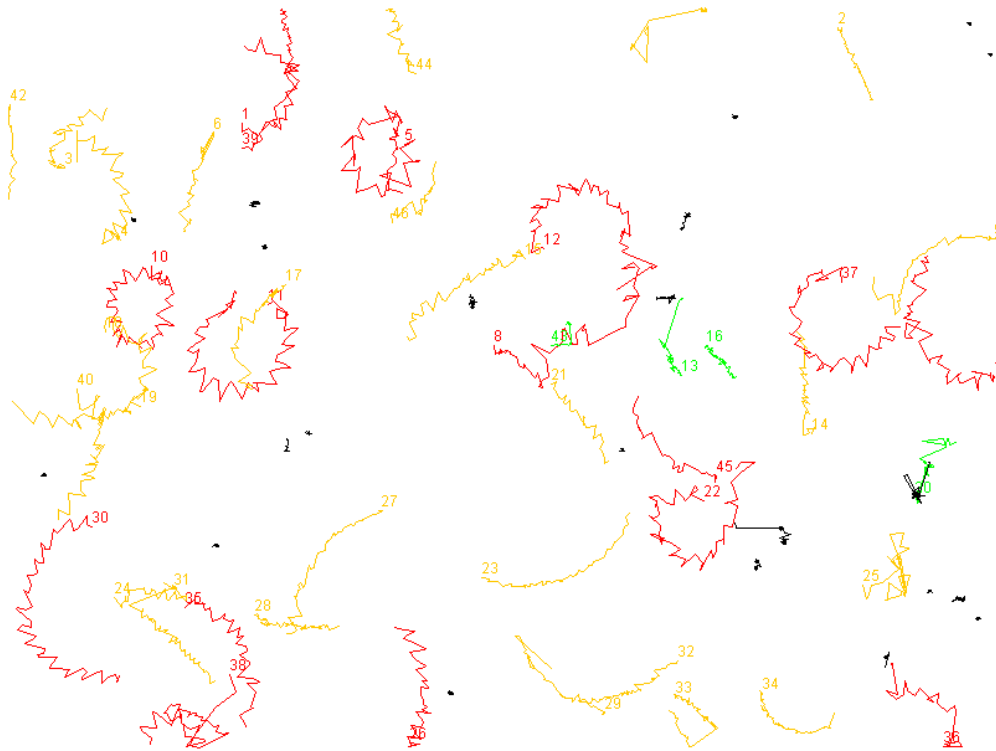

555

556

557 *Figure 3.* “Paths” window. Each spermatozoon analyzed by the plugin is assigned a
 558 number, following the order of the “results” window and a color, depending on the VAP.
 559 Red, rapid cells with VAP higher than the value inserted in the input field “i”; yellow,
 560 medium cells with VAP between the value in the input field “i” and “h”; green, slow cells,
 561 with VAP lower that the value inserted in the input field “h”. Black tracks are those of non
 562 motile cells (velocities beneath).

563

564

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

565 Supplementary file 1.

566 Bland Altman plots representing agreement between parameters measured by IVOS Hamilton-
567 Thorne CASA and CASA_bgm plugin. Each point represent a sample, measured with both
568 instruments. Y axis expresses difference in means, while X axis expresses the average between the
569 two measurements. The external lines represents ± 2 SD.


570

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

571 Total motility(TM) Bland Altman's plot

572

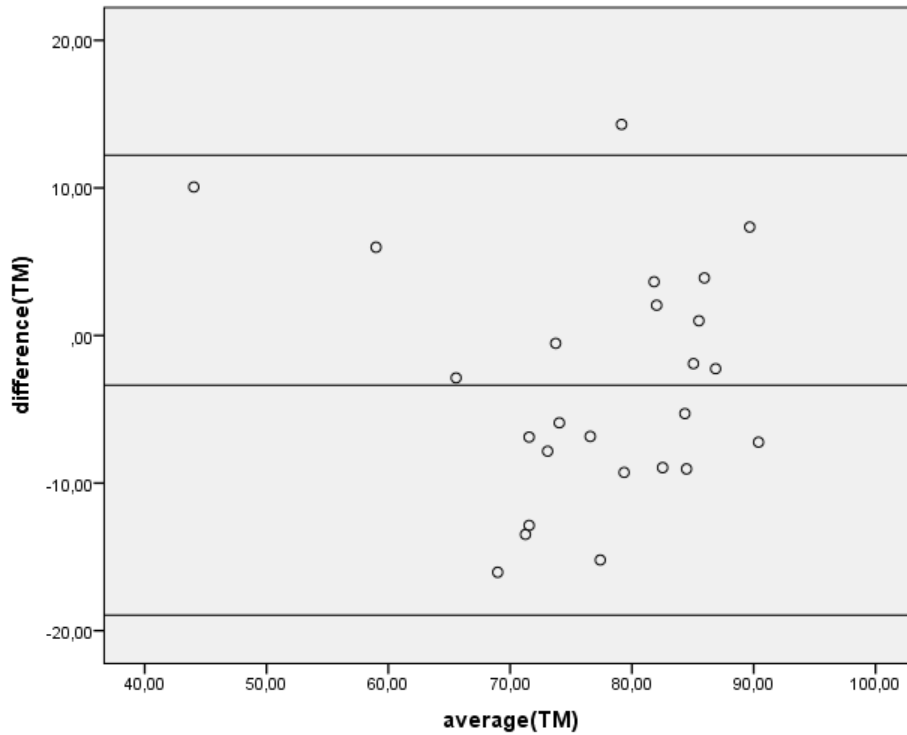

573

574

575


576

577 Progressive motility(PM) Bland Altman's plot

578

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

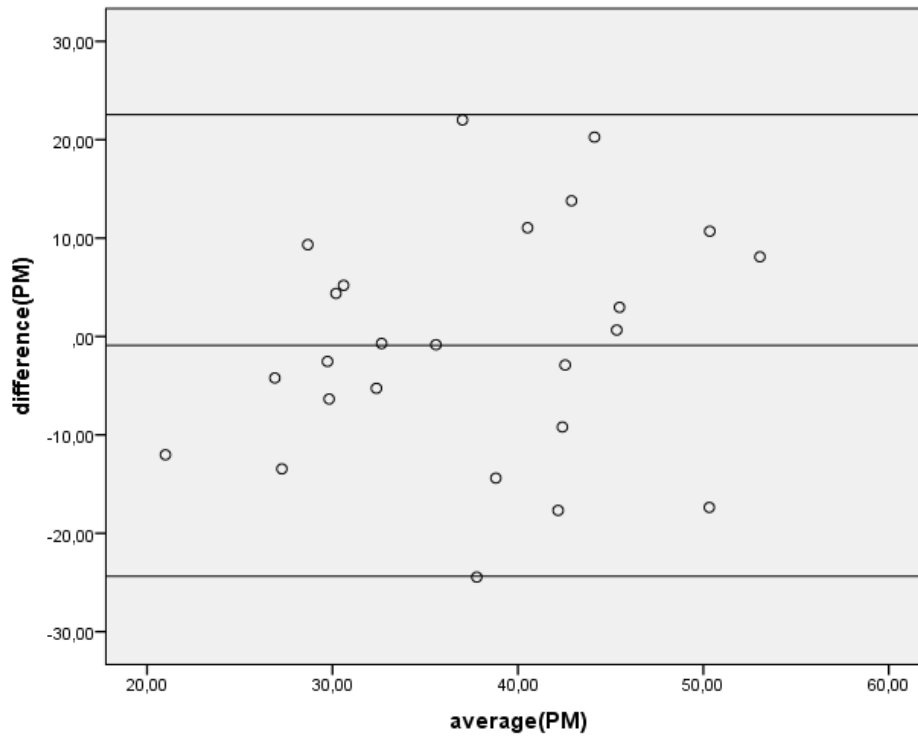

579


580

581 Linear velocity (VCL) Bland Altman's plot

582

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

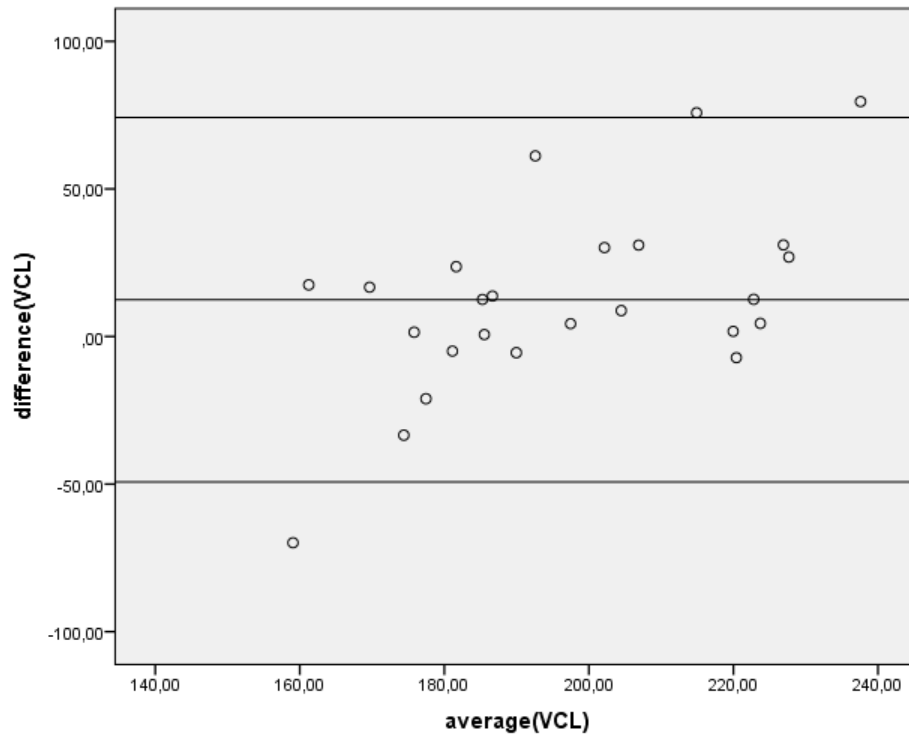

583

584

585


586

587 Mean velocity (VAP) Bland Altman's plot

588

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

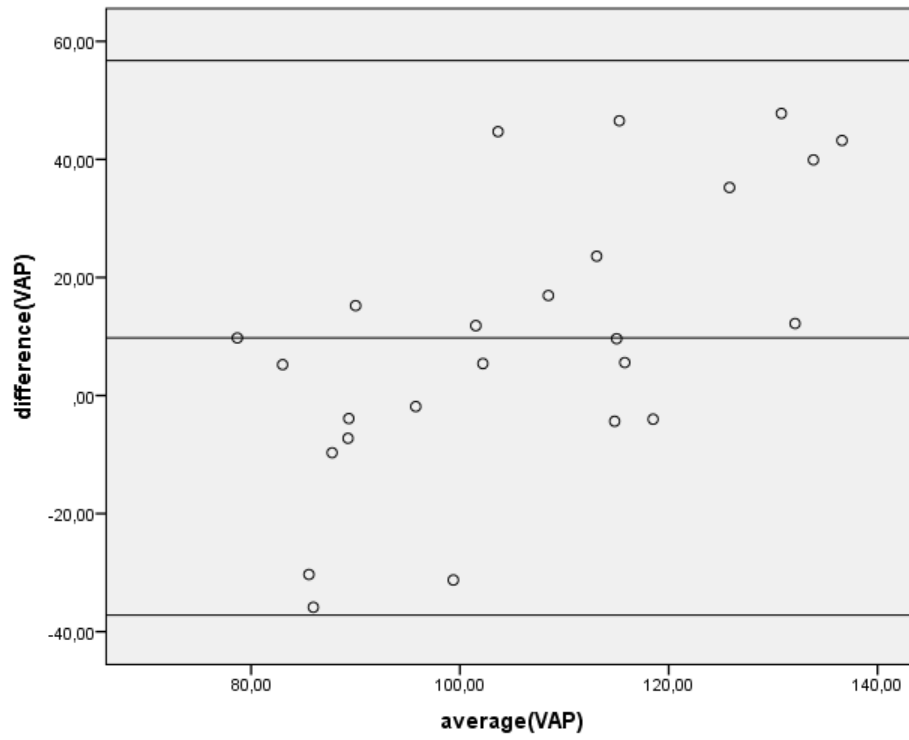

589


590

591 Linear velocity (VSL) Bland Altman's plot

592

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

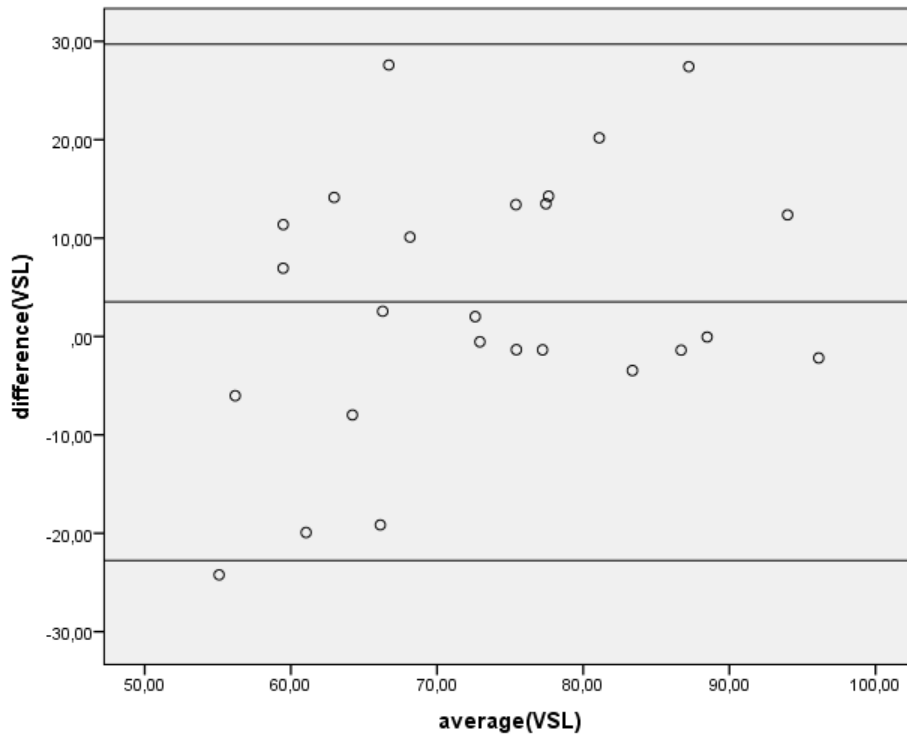

593

594

595


596

597 Linearity (LIN) Bland Altman's plot

598

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)


When citing, please refer to the published version.

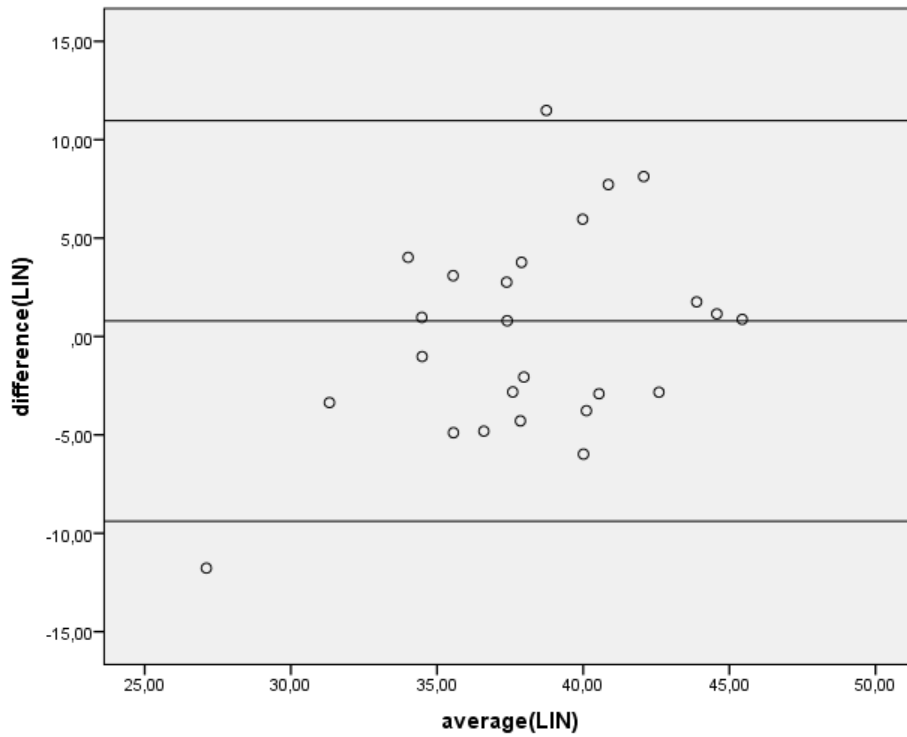

599

600 Straightness (STR) Bland Altman's plot

601

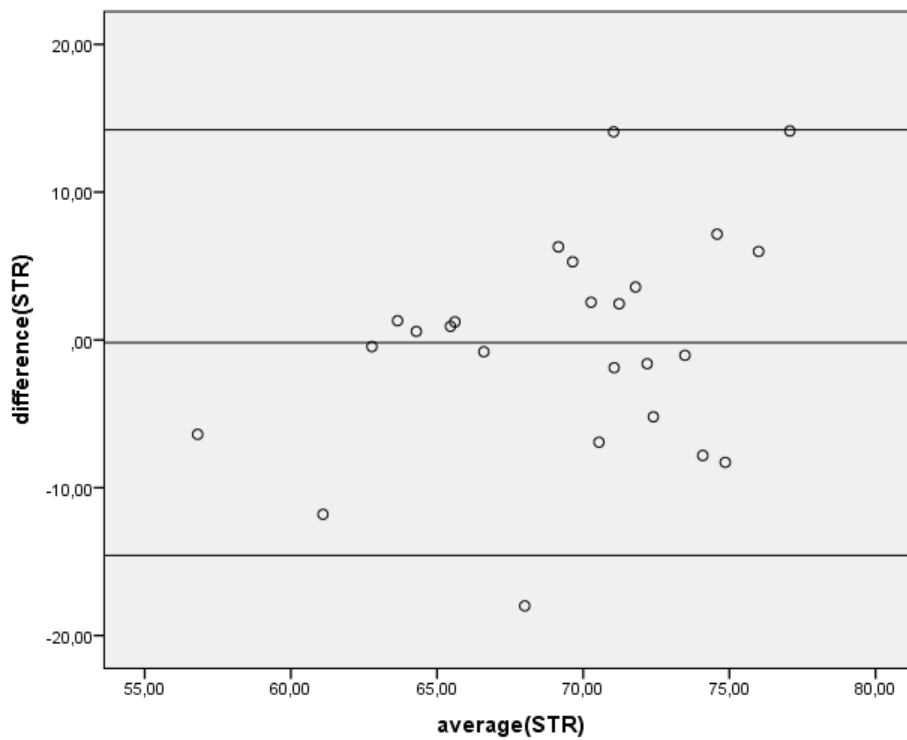

602

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.


603

604

605

606 Beat Cross Frequency (BCF) Bland Altman's plot

607

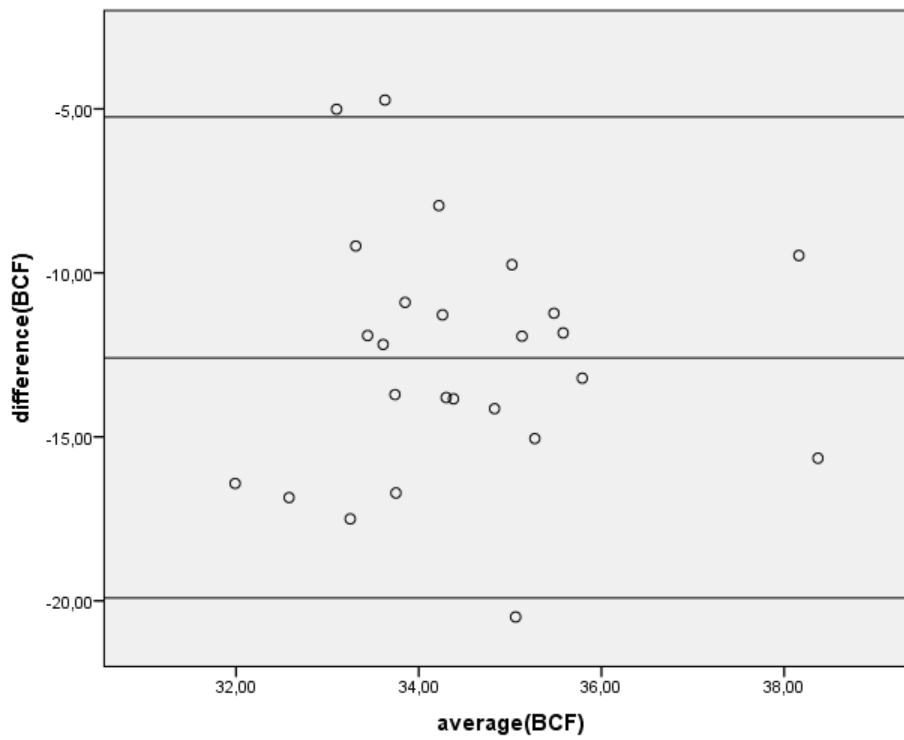


608

609 Amplitude of lateral head displacement (ALH) Bland Altman's plot

610

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

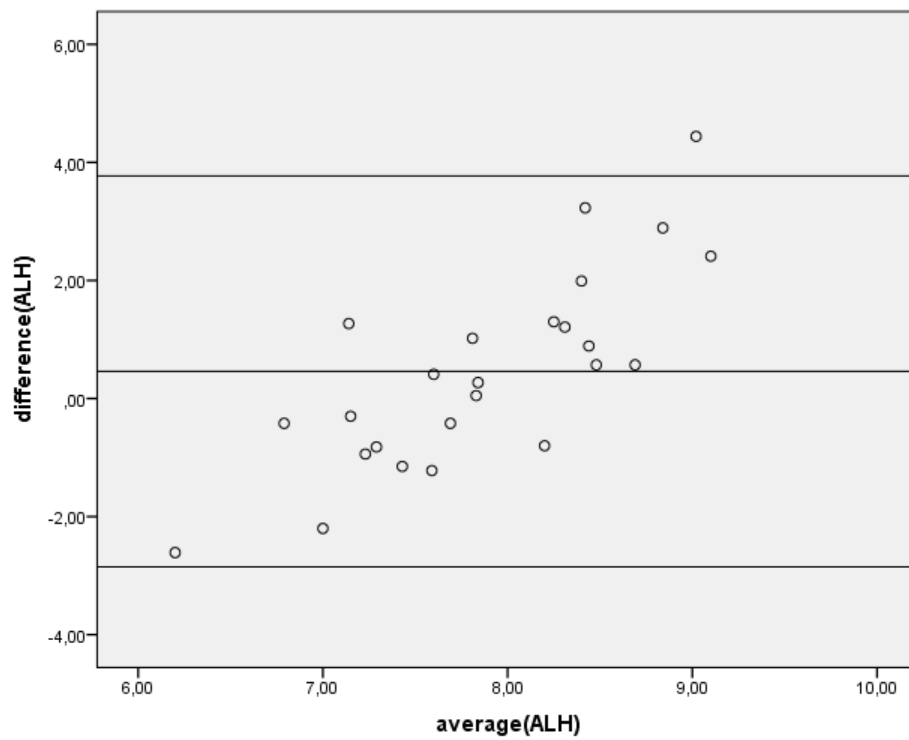

611

612

613

614

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

615 Declaration of intent.

616

617 The CASA_BGM plugin was obtained by modifying and renewing the “casa” plugin Computer Assisted
618 Sperm Analyzer designed by JG Wilson-Leedy JG and RL Ingermann and owned by the Regents of the
619 University of California and the Howard Hughes Medical Institute.

620

621 The plugin is subjected to the following conditions and terms of use:

622

623 Wilson-Leedy JG, Ingermann RL, Development of a novel CASA system based on open source software for
624 characterization of zebrafish sperm motility parameters, *Theriogenology* (2006),
625 doi:10.1016/j.theriogenology.2006.10.003.

626 Copyright © 2003 The Regents of the University of California and the Howard Hughes Medical Institute.

627 All Rights Reserved.

628 Permission to use, copy, modify, and distribute this software and its documentation for educational, research
629 and non-profit purposes, without fee, and without a written agreement is hereby granted, provided that the
630 above copyright notice, this paragraph and the following three paragraphs appear in all copies.

631 Permission to incorporate this software into commercial products may be obtained by contacting the Office of
632 Technology Management at the University of California San Francisco [Sunita Rajdev, Ph.D., Licensing
633 Officer, UCSF Office of Technology Management. 185 Berry St, Suite 4603, San Francisco, CA 94107].

634 This software program and documentation are copyrighted by The Regents of the University of California
635 acting on behalf of the University of California San Francisco via its Office of Technology Management and
636 the Howard Hughes Medical Institute (collectively, the Institution). The software program and documentation
637 are supplied "as is", without any accompanying services from the Institution. The Institution does not warrant
638 that the operation of the program will be uninterrupted or error-free. The end-user understands that the program
639 was developed for research purposes and is advised not to rely exclusively on the program for any reason.

640 IN NO EVENT SHALL THE INSTITUTION BE LIABLE TO ANY PARTY FOR DIRECT, INDIRECT,
641 SPECIAL, INCIDENTAL, OR CONSEQUENTIAL DAMAGES, INCLUDING LOST PROFITS, ARISING
642 OUT OF THE USE OF THIS SOFTWARE AND ITS DOCUMENTATION, EVEN IF THE INSTITUTION
643 HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGE. THE INSTITUTION
644 SPECIFICALLY DISCLAIMS ANY WARRANTIES, INCLUDING, BUT NOT LIMITED TO, THE
645 IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE.
646 THE SOFTWARE PROVIDED HEREUNDER IS ON AN "AS IS" BASIS, AND THE INSTITUTION HAS
647 NO OBLIGATIONS TO PROVIDE MAINTENANCE, SUPPORT, UPDATES, ENHANCEMENTS, OR
648 MODIFICATIONS.

649

650

651 The purpose of our work is to implement an open source tool and share with the international research
652 community our findings and, possibly, start collaborations for further implementations. We neglect and reject
653 any commercial use of our plugin.

654

655

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

656 Brief instructions for analysis with ImageJ CASA_BGM plugin

657

658 Plugin installation

659 We report the original instruction from Wilson Leedy and Ingermann

660 “The plugin must first be downloaded to the computer’s plugins folder and compiled
661 (Plugins->Compile and Run, locate the file and open, see
662 <http://rsb.info.nih.gov/ij/docs/menus/plugins.html> for more detailed instruction).
663 Running the plugin will result in initiation of a dialog box where parameters for analysis
664 may be entered (and must be entered for each analysis performed - we recommend use of
665 a macro to input these values, macros can then be saved with particular settings for a
666 specific species). Macros can be recorded by opening the macro recorder (Plugins->Macros-
667 >Record), and performing the analysis as normal. Clicking Create will open a new window
668 with the text of the macro, running this macro will open the plugin, input the previously
669 used values, and run the plugin. See
670 <http://rsb.info.nih.gov/ij/docs/menus/plugins.html#macros> and
671 <http://rsb.info.nih.gov/ij/developer/macro/macros.html#recorder> for more detailed
672 instructions regarding macro recording.”

673

674 Import a video in Image J and analysis

675

676 After saving videos of sperm samples, these should be converted in .avi format.

677 To import the video into Image J after launching the software, choose *File>Import>Avi...*
678 and chose the file from the correct folder.

679 A dialog box opens and it should be indicated to import frames from 60 to 120 and to
680 convert the image to greyscale.

681 The video opens and the threshold should then be adjusted. Use Image->Adjust-
682 >Threshold file menu. Adjust the sliders to select spermatozoa (red) and avoid selecting
683 any background image (the background should be white). By clicking “Apply” the image is
684 converted into black and white (black spermatozoa and white background).

685 Launch the plugin and fill each field with the appropriate values (see the main article for
686 stallion) or alternatively create and run a specific Macro.

687

688

689

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.