



ALMA MATER STUDIORUM
UNIVERSITÀ DI BOLOGNA

ARCHIVIO ISTITUZIONALE DELLA RICERCA

Alma Mater Studiorum Università di Bologna Archivio istituzionale della ricerca

Bioelectrical impedance analysis versus reference methods in the assessment of body composition in athletes

This is the final peer-reviewed author's accepted manuscript (postprint) of the following publication:

Published Version:

Campa F., Gobbo L.A., Stagi S., Cyrino L.T., Toselli S., Marini E., et al. (2022). Bioelectrical impedance analysis versus reference methods in the assessment of body composition in athletes. EUROPEAN JOURNAL OF APPLIED PHYSIOLOGY, 122(3), 561-589 [10.1007/s00421-021-04879-y].

Availability:

This version is available at: <https://hdl.handle.net/11585/861948> since: 2023-10-31

Published:

DOI: <http://doi.org/10.1007/s00421-021-04879-y>

Terms of use:

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>).
When citing, please refer to the published version.

(Article begins on next page)

This is the final peer-reviewed accepted manuscript of:

Campa F, Gobbo LA, Stagi S, et al (2022) Bioelectrical impedance analysis versus reference methods in the assessment of body composition in athletes. Eur J Appl Physiol 122:561–589. <https://doi.org/10.1007/s00421-021-04879-y>

The final published version is available online at:

<https://doi.org/10.1007/s00421-021-04879-y>

Terms of use:

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)

When citing, please refer to the published version.

[Click here to view linked References](#)

1 **Bioelectrical Impedance Analysis versus Reference Methods in the Assessment of Body Composition in Athletes A**

2 ~~Systematic Review~~

3
4 3

5
6 4 Francesco Campa¹, Luis Alberto Gobbo², Silvia Stagi³, Leticia Trindade Cyrino, Stefania Toselli⁴, Elisabetta Marini³,

7
8 5 Giuseppe Coratella^{5*}

9
10 6

11
12 7 ¹ Department for Life Quality Studies, Università degli Studi di Bologna, Rimini, Italy. ORCID iD: [https://orcid.org/0000-](https://orcid.org/0000-0002-3028-7802)

13
14 8 [0002-3028-7802](https://orcid.org/0002-3028-7802)

15
16 9 ² Department of Physical Education, São Paulo State University, Presidente Prudente, SP, Brazil. ORCID iD:

17
18 10 <https://orcid.org/0000-0001-7523-9102>

19
20 11 ³ Department of Life and Environmental Sciences, University of Cagliari, Cittadella Universitaria, Monserrato, Cagliari,

21
22 12 Italy. ORCID iD (Marini): <https://orcid.org/0000-0001-8779-8745>. ORCID iD (Stagi): [https://orcid.org/0000-0002-6469-](https://orcid.org/0000-0002-6469-4334)

23
24 13 [4334](https://orcid.org/0000-0002-6469-4334).

25
26 14 ⁴ Department of Biomedical and Neuromotor Sciences, Università degli Studi di Bologna, Bologna, Italy. ORCID iD:

27
28 15 <https://orcid.org/0000-0001-5478-2499>

29
30 16 <https://orcid.org/0000-0002-7980-6749>

31
32 17 ⁵ Department of Biomedical Sciences for Health, Università degli Studi di Milano, Milan, Italy. ORCID iD:

33
34 18 <https://orcid.org/0000-0001-7523-9102>

35
36 19 * Corresponding author: Giuseppe Coratella

37
38 20 Department of Biomedical Sciences for Health, Università degli Studi di Milano, Milan, Italy. Mail address: via Giuseppe

39
40 21 Colombo 71, 20133, Milano, Italy.

41
42 22 Email address: Giuseppe.coratella@unimi.it

43
44 23

45
46 24 **Funding:** This research project received no external funding.

47
48 25 **Conflicts of interest/Competing interests:** The authors declare no conflict of interest. Availability of data and material:

49
50 26 Not applicable

51
52 27 **Ethics approval:** Not applicable

53
54 28

55
56 29

57
58 30

59
60 31

61
62
63
64
65

32 **Abstract**

1
2 33 The present systematic review aimed to compare the accuracy of Bioelectrical Impedance Analysis (BIA) and
3
4 34 Bioelectrical Impedance Vector Analysis (BIVA) vs. reference methods for the assessment of body composition in
5
6 35 athletes. Studies were identified based on a systematic search of internationally electronic databases (PubMed and Scopus)
7
8 36 and hand searching of the reference lists of the included studies. In total, 42 studies published between 1988 and 2021
9
10 37 were included. The methodological quality was assessed using the Quality Assessment Tool for Observational Cohort
11
12 38 and Cross-sectional Studies as recommended by the National Institute of Health. Twenty-three studies had an overall
13
14 39 good rating in terms of quality, while 13 were rated as fair and six as poor, resulting in a low to moderate risk of bias. Fat
15
16 40 mass was inconsistently determined using BIA vs. the reference methods, regardless of the BIA-technology. When using
17
18 41 the foot to hand technology with predictive equations for athletes, a good agreement between BIA and the reference
19
20 42 methods was observed for fat-free mass, total body, intra and extra cellular water. However, an underestimation in fat-
21
22 43 free mass and body fluids was found when using generalized predictive equations. Classic and *Specific* BIVA represented
23
24 44 a valid approach for assessing body fluids (Classic BIVA) and percentage of fat mass (*Specific* BIVA). The present
25
26 45 systematic review suggests that BIA and BIVA can be used for assessing body composition in athletes, provided that
27
28 46 foot-to-hand technology, predictive equations, and BIVA references for athletes are used.

29
30 47
31
32 48 **Keywords:** Bioimpedance vector analysis; Classic BIVA; *Specific* BIVA; Phase angle; Tolerance ellipses; Resistance
33
34 49 training; Nutrition

35
36 50
37
38 51
39
40 52
41
42 53
43
44 54
45
46 55
47
48 56
49
50 57
51
52 58
53
54 59
55
56 60
57
58 61
59
60 62
61
62
63
64
65

63 **Abbreviations**

| | | |
|----|----|--|
| 1 | | |
| 2 | 64 | BIA Bioelectrical impedance analysis |
| 3 | | |
| 4 | 65 | BIVA Bioelectrical impedance vector analysis |
| 5 | | |
| 6 | 66 | BIS Bioelectrical spectroscopy analysis |
| 7 | | |
| 8 | 67 | DXA Dual-energy X-ray absorptiometry |
| 9 | | |
| 10 | 68 | ECW Extracellular water |
| 11 | | |
| 12 | 69 | FM Fat mass |
| 13 | | |
| 14 | 70 | FFM Fat free mass |
| 15 | | |
| 16 | 71 | ICW Intracellular water |
| 17 | | |
| 18 | 72 | LST Lean soft tissue |
| 19 | | |
| 20 | 73 | R Resistance |
| 21 | | |
| 22 | 74 | Xc Reactance |
| 23 | | |
| 24 | 75 | TBW Total body water |
| 25 | | |
| 26 | 76 | UWW Underwater weighting |
| 27 | | |
| 28 | 77 | 4C Four compartment model |
| 29 | | |
| 30 | 78 | |
| 31 | | |
| 32 | 79 | |
| 33 | | |
| 34 | 80 | |
| 35 | | |
| 36 | 81 | |
| 37 | | |
| 38 | 82 | |
| 39 | | |
| 40 | 83 | |
| 41 | | |
| 42 | 84 | |
| 43 | | |
| 44 | 85 | |
| 45 | | |
| 46 | 86 | |
| 47 | | |
| 48 | 87 | |
| 49 | | |
| 50 | 88 | |
| 51 | | |
| 52 | 89 | |
| 53 | | |
| 54 | 90 | |
| 55 | | |
| 56 | 91 | |
| 57 | | |
| 58 | 92 | |
| 59 | | |
| 60 | 93 | |
| 61 | | |
| 62 | | |
| 63 | | |
| 64 | | |
| 65 | | |

94 **Introduction**

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20
21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65

Body composition describes the amount of the various components of the human body, such as fat (FM) and muscle mass or body fluids (Heymsfield et al. 2005). However, the assessment of body composition through direct procedures is not possible in humans (Heymsfield et al. 2005). For this reason, a number of indirect methods have been developed and implemented over the years, allowing to assess a wide range of body composition parameters (Heymsfield et al. 2005). Among these methods, some are considered as the gold standard for certain parameters, such as the dilution techniques for the body fluids assessment (Heymsfield et al. 2005). Other methods including energy X-ray absorptiometry (DXA), underwater weighing (UWW), air displacement plethysmography, magnetic resonance, and computed tomography are also classified as indirect approaches and used as reference methods in the body composition evaluation (Heymsfield et al. 2005).

However, most of the aforementioned techniques are expensive and require long procedures and highly specialized personnel (Campa et al. 2021b). For this reason, double-indirect methods have been implemented for obtaining estimations derived from indirect methods such as DXA, UWW or dilution techniques through validated regression equations. Over the recent years, ~~the~~ bioelectrical impedance analysis (BIA) has been identified as a possible alternative for assessing body composition. Although BIA is classified as a double-indirect approach, being noninvasive, portable, relatively low-cost, and technologically friendly, its use has gained attention in clinical and practical, as well as in research contexts (Lukaski and Raymond-Pope 2021). BIA is based on the different impedance of fat and lean tissues when a weak electric current flows through the body and several technologies have been designed and commercialized to date. These technologies include hand to hand, leg to leg, foot to hand direct or segmental approach, implying profound differences in both testing procedures (e.g., body position and electrodes placement) and final outcomes (Dellinger et al. 2021; Stratton et al. 2021). The hand to hand technology measures the upper body impedance, the foot to foot measures the lower body impedance, and the foot to hand measures the right hemisoma impedance, all estimating the remaining body sections through dedicated algorithms; on the contrary, the direct segmental technology measures the whole-body impedance (Campa et al. 2021b). Based on these four technologies, many devices have been produced by the manufacturers, working at a wide range of sampling frequency (from 1 to 1000 kHz), albeit the 50 kHz frequency has been identified as the most appropriate for measuring bioimpedance in humans (Kyle et al. 2004a, b).

The traditional BIA approach allows the quantification of both absolute (kg or L) or relative amount (%) of a number of body composition parameters through predictive equations, thanks to the different conductance properties of each

125 biological tissue. In fact, FM shows poor conductive proprieties, while fat-free mass (FFM), including the lean soft tissue
126 (LST) and body fluids, is a good electrical conductor (Lukaski and Piccoli 2012). Following the procedures, the devices
127 may either provide the quantitative estimation of body composition parameters using predictive equations set by the
128 manufacturer or provide the raw resistance (R) and reactance (Xc) to be inserted into specific formulas up to the operator
129 (Campa et al. 2021b). In this regard, most of the formulas have been developed for non-athletic populations, and formulas
130 for athletes have been designed recently (Campa et al. 2021b). This may have an impact on the final outcomes, as shown
131 in athletes samples (Pichard et al. 1997; Houtkoop et al. 2001; Matias et al. 2016a,b; Deminice et al. 2016; Shiose et al.
132 2020; Coratella et al. 2021). However, these studies examined the difference in body composition outcomes comparing
133 BIA vs. reference methods considering only a single BIA technology or a given body composition parameter (e.g., FM
134 and FFM or body fluids) in athletes. Notwithstanding, many studies have compared the BIA vs. reference methods in
135 athletes using different BIA-technologies, predictive equations, and devices. All these studies have not been
136 systematically reviewed so far, in order to provide a comprehensive overview of the literature.

137
138 A further approach when using bioimpedance parameters is the bioelectrical impedance vector analysis (BIVA), proposed
139 by Piccoli et al. (Piccoli et al. 1994) in 1994 and modified by Buffa et al. (Buffa et al. 2013) in 2013. The initial approach
140 (Classic BIVA) consists of the simultaneous evaluation of R and Xc adjusted for the stature, plotting them as a vector
141 within a graph (Piccoli et al. 1994). The later approach (*Specific BIVA*), consists of the concurrent adjustment of R and
142 Xc for the stature and for the cross-sectional area of the arm, waist, and calf (Buffa et al. 2013). Classic and *Specific*
143 BIVA were developed with the aim to determine total body water (TBW) and %FM, respectively. The change in vector
144 length reflects the change in TBW (Classic BIVA) or %FM (*Specific BIVA*), while the lateral displacement of the vector
145 reflects the bioelectrical phase angle for both BIVA approaches, graphically represented as the angle between the vector
146 and the x-axis (Stahn et al. 2012). Particularly, the phase angle has been proposed as an indicator of cellular health, cell
147 membrane integrity (Stahn et al. 2012; Lukaski and Raymond-Pope 2021) and faithfully reflects the
148 intracellular/extracellular water (ICW/ECW) ratio (Marini et al. 2020; Campa et al. 2021b). As such, BIVA allows a
149 qualitative assessment of body composition, avoiding the use of prediction equations to estimate the different parameters.
150 Additionally, although BIVA does not quantify each component, the vector position can be evaluated within tolerance
151 ellipses drawn for each population, representing their percentile within that population distribution (Campa et al. 2019).
152 The use of BIVA in athletes has been implemented quite recently, and a few studies have assessed body composition in
153 athletes using both BIVA and reference methods. Some authors have systematically reviewed the use of BIVA in sports
154 practice (Castizo-Olier et al. 2018), albeit they did not focus on the comparison of BIVA vs. reference methods. In this
155 regard, this was not possible at that time, given that the first studies comparing BIVA vs. reference method in athletes

156 was only published in 2020 (Campa et al. 2020; Marini et al. 2020). Figure 1 depicts the key concepts of BIA and the
157 application of BIVA.

158
159 ***Insert Figure 1 next here***

160
161 Therefore, the main purposes of the present systematic review were to summarize the results of studies that compared i)
162 BIA vs. reference methods in the estimation of body composition parameters in athletes and ii) BIVA vs. reference
163 methods in the qualitative assessment of body composition parameters in athletes. Furthermore, we aimed to provide
164 appropriate strategies to assess body composition in athletes using BIA or BIVA, considering the different technologies
165 and predictive equations.

166 167 **Methods**

168 169 Search strategy and eligibility criteria

170 The present study was carried out following the preferred reporting items for systematic reviews and meta-analyses
171 (PRISMA) guidelines (Page et al. 2021). The bibliographic search was performed on August 15th, 2021, using Scopus
172 and PubMed online databases. The search query was applied to the source title, abstract, and keywords, and included
173 combinations of at least one of the terms identifying body composition, with at least one of the terms identifying the
174 bioimpedance techniques applied, a term on the reference technique, and a term on the field of application. The resulting
175 search query was:

176 (“body composition” OR “fat mass” OR “fat free mass” OR “muscle mass” OR “lean mass” OR “total body water” OR
177 “extracellular water” OR “intracellular water” OR FM OR FFM OR TBW OR ECW OR ICW) AND (BIA OR
178 bioimpedance OR “bioelectrical impedance” OR BIVA OR “bioelectrical impedance vector analysis” OR “vector
179 analysis” OR biavector) AND (DXA OR DEXA OR densitometry OR imaging OR CT OR tomography OR MRI OR
180 MRT OR magnetic OR RMT OR RM OR “dilution techniques” OR “deuterium dilution” OR “isotope dilution” OR
181 UWW OR hydrodensitometry OR “underwater weight” OR "BOD POD" OR ADP OR “air-displacement
182 plethysmography” OR “criterion method” OR “standard technique” OR “direct technique” OR “reference technique”)
183 AND (sport OR athletes). To identify additional relevant papers, hand searching of the reference lists of the included
184 papers was performed.

185
186 The inclusion criteria were:

- 187
- Peer-reviewed articles that assessed body composition in athletes involved in individual or team sports using BIA or BIVA and reference techniques.
- 188
- Accessible in English full text.
- 189
- Individuals aged above 16 years, and with no chronic diseases or health problems.
- 190

191 The exclusion criteria were:

- Reviews and case studies.
 - Articles aimed to develop predictive equations without a cross-validation group.
- 192
- 193
- 194
- 195

Study selection and data processing

196 Based on the initial titles retrieved, duplicates were removed. Abstracts identified from the literature searches were
197 screened for potential inclusion by two authors (F.C. and G.C.) and a third author (L.G.) when there was a disagreement
198 between the first two. Data extraction included information about each article, such as: authors, year, study design,
199 participants' information (sex, age), ~~type of~~ sports code, bioimpedance methodology and devices, reference technique,
200 outcome measures and main results.

Quality assessment

203 Methodological quality was assessed using the Quality Assessment Tool for Observational Cohort and Cross-sectional
204 Studies in observational studies (NIH 2014) recommended by the National Institute of Health, U.S. Department of Health
205 and Human Services. The tool consists of 14 criteria that are used to assess quality, including whether the population
206 studied was clearly specified and defined, whether the outcome assessors were blinded, and an assessment of the
207 participation rate. The criteria were classified as “yes”, “no”, “unclear”, or “not applicable”. Quality rates were good, fair,
208 or poor as judged by two independent observers (F.C. and L.G.) following the instructions given by the National Institute
209 of and Human Services.

Results

Search outcomes

214 The literature search resulted in 554 articles. After removal of duplicates (n= 242) and abstract screening, 43 studies were
215 considered relevant. After the full text screening, 11 were further excluded, so that a total of 32 studies fully met the
216 eligibility criteria. Ten additional studies were included after a hand searching of the reference lists of the included articles.

217 The PRISMA flow chart is shown in Figure 1. Finally, 42 studies published between 1988 and 2021 were considered. Out
218 of these 42 articles, 37 presented a cross-sectional and five a longitudinal study design.

219
220 ***Insert Figure 2 next here***

221 222 Participants

223 A total of 2978 subjects (1962 men and 1016 women) participated in the selected studies. Regarding sports code, N=534
224 participants were involved in team sports, N=339 in individual sports, while the exact number of subjects for each sport
225 modality was not reported for N=2105 participants.

226 227 Risk of bias

228 The risk of bias resulted as low to moderate, as summarized in Supplementary Table 1. Measurement procedures (e.g.,
229 electrodes placement, hydration status, food and fluid intake before the test or time from the last exercise) of BIA were
230 sometimes not completely described. Furthermore, the predictive equations used to estimate body composition parameters
231 were not always reported. Twenty-three studies had an overall good rating in terms of quality, while 13 were rated as fair
232 and 6 as poor (Table S1).

233 234 Bioelectrical devices and technologies

235 The selected articles included different devices and technologies as shown in Figure 2. Considering the four different
236 technologies, 4 articles used the hand to hand (Esco et al. 2011; Loenneke et al. 2013; Graybeal et al. 2020; Syed-Abdul
237 et al. 2021), 6 the leg to leg (Civar et al. 2003, 2006; Dixon et al. 2005; Loenneke et al. 2013; Domingos et al. 2019;
238 Graybeal et al. 2020), 29 the foot to hand (Birzniece et al. 2015; Colville et al. 1989; Lukaski et al. 1990; Kirkendall et
239 al. 1991; Hortobágyi et al. 1992; Pichard et al. 1997; Williams and Bale 1998; Fornetti et al. 1999; De Lorenzo et al.
240 2000; Houtkoopr et al. 2001; Andreoli et al. 2004; Svantesson et al. 2008; Company and Ball 2010; Matias et al. 2016a,
241 b, 2021; Deminice et al. 2016; Krzykała et al. 2016; Arias Téllez et al. 2019; Campa et al. 2020, 2021; Marini et al. 2020;
242 Graybeal et al. 2020; Silva et al. 2020; Sardinha et al. 2020; Shiose et al. 2020; Stagi et al. 2021; Francisco et al. 2021;
243 Coratella et al. 2021), and 9 the direct segmental technology (Loenneke et al. 2012, 2013; Esco et al. 2015; Krzykała et
244 al. 2016; Raymond et al. 2018; Brewer et al. 2019; Hartmann Nunes et al. 2020; Graybeal et al. 2020; Lee et al. 2021).
245 Particularly, more than one technology was used in some studies and for each technology, different devices were used.
246 Considering the dependent variables, 30 articles (Birzniece et al. 2015; Colville et al. 1989; Lukaski et al. 1990; Kirkendall
247 et al. 1991; Hortobágyi et al. 1992; Pichard et al. 1997; Williams and Bale 1998; Fornetti et al. 1999; De Lorenzo et al.

248 2000; Houtkoopr et al. 2001; Civar et al. 2003, 2006; Andreoli et al. 2004; Dixon et al. 2005; Svantesson et al. 2008;
249 Company and Ball 2010; Esco et al. 2011, 2015; Loenneke et al. 2012, 2013; Krzykała et al. 2016; Raymond et al. 2018;
250 Arias Téllez et al. 2019; Domingos et al. 2019; Brewer et al. 2019; Hartmann Nunes et al. 2020; Graybeal et al. 2020;
251 Sardinha et al. 2020; Lee et al. 2021; Matias et al. 2021; Syed-Abdul et al. 2021) assessed FM and FFM comparing BIA
252 with reference methods, although seven additional studies used more than one technology, resulting in 37 comparisons.
253 A total of 7 studies (Birzniece et al. 2015; Matias et al. 2016b, a; Deminice et al. 2016; Shiose et al. 2020; Coratella et al.
254 2021; Francisco et al. 2021) assessed body fluids comparing BIA with reference methods, using the foot to hand
255 technology. A total of 5 articles (Campa et al. 2020, 2021a; Marini et al. 2020; Silva et al. 2020; Stagi et al. 2021) assessed
256 body composition comparing BIVA with reference methods, using the foot to hand technology.

257
258 ***Insert Figure 3 next here***
259

260 BIA vs. reference methods: FM and FFM

261
262 Table 1 shows the study design, demographic information, bioimpedance methodology, reference methods, and the main
263 results for each study. Considering the 16 studies that used a foot to hand technology for assessing FM, eight (Colville
264 et al. 1989; Hortobágyi et al. 1992; Pichard et al. 1997; Williams and Bale 1998; Boileau and Horswill 2000; Houtkoopr
265 et al. 2001; Andreoli et al. 2004; Company and Ball 2010) showed an overestimation of the %FM obtained by BIA, five
266 studies an underestimation of %FM (Lukaski et al. 1990; De Lorenzo et al. 2000; Arias Téllez et al. 2019) and FM
267 (Svantesson et al. 2008; Birzniece et al. 2015), while three studies showed an agreement in the estimated %FM (Pichard
268 et al. 1997; Krzykała et al. 2016) and FM (Graybeal et al. 2020). Birzniece et al. (Birzniece et al. 2015) observed both a
269 cross-sectional and longitudinal underestimation of %FM obtained by BIA. Of these studies, only seven (Colville et al.
270 1989; Lukaski et al. 1990; Pichard et al. 1997; De Lorenzo et al. 2000; Houtkoopr et al. 2001; Andreoli et al. 2004;
271 Company and Ball 2010) reported the predictive equations used. Considering the 10 studies that used a foot to hand
272 technology for assessing FFM, four studies showed a good agreement between BIA and reference methods (Lukaski et
273 al. 1990; Fornetti et al. 1999; Graybeal et al. 2020; Matias et al. 2021), three studies showed an underestimation (Colville
274 et al. 1989; Hortobágyi et al. 1992; Pichard et al. 1997) and three studies showed an overestimation of FFM (De Lorenzo
275 et al. 2000; Svantesson et al. 2008; Birzniece et al. 2015). Birzniece et al. (Birzniece et al. 2015) observed both a cross-
276 sectional and longitudinal overestimation of FFM obtained by BIA. Of these studies, only seven (Colville et al. 1989;
277 Lukaski et al. 1990; Pichard et al. 1997; Fornetti et al. 1999; De Lorenzo et al. 2000; Houtkoopr et al. 2001; Matias et al.
278 2021) reported the predictive equations used. LST of the arm and legs was estimated by only one study (Sardinha et al.

279 2020), which showed an excellent agreement between BIA and the reference method and reported the predictive
280 equations.

281
282 Nine studies used a direct segmental technology for assessing FM, albeit Lee et al. (Lee et al. 2021) utilized three different
283 devices for a total of 11 comparisons. Six studies reported an overestimation of FM (Brewer et al. 2019; Hartmann Nunes
284 et al. 2020; Graybeal et al. 2020; Lee et al. 2021) and %FM (Loenneke et al. 2013; Lee et al. 2021). Of these six studies,
285 one used a regional approach for investigating the legs FM (Brewer et al. 2019), and one assessed the visceral FM
286 (Hartmann Nunes et al. 2020). Three studies (Esco et al. 2015; Krzykała et al. 2016; Raymond et al. 2018) showed an
287 underestimation of %FM, and one of them used a regional approach measuring the arms and legs FM (Raymond et al.
288 2018), three studies (Raymond et al. 2018; Brewer et al. 2019; Graybeal et al. 2020) showed no difference between BIA
289 and the reference methods. The study by Graybeal et al. (Graybeal et al. 2020) found higher %FM only in men, while
290 they reported a good agreement in women. None of these nine studies using the direct segmental technique reported the
291 equations. Five studies used a direct segmental technology for assessing FFM. Four studies showed an underestimation
292 compared with the reference method. Of these four studies, Graybeal et al. (Graybeal et al. 2020) found this result only
293 in men, while Raymond et al. (Raymond et al. 2018) referred to arms and Brewer et al. (Brewer et al. 2019) to arms and
294 legs FFM. Two studies reported an overestimation in FFM (Loenneke et al. 2012; Esco et al. 2015), and two studies
295 reported no difference in the FFM, but only when measuring women (Graybeal et al. 2020) or the trunk FFM (Raymond
296 et al. 2018). None of these five studies using the direct segmental technique reported the equations. Esco et al. (Esco et
297 al. 2015) was the only study that using a regional approach for assessing arm, leg, and trunk LST, reported a good
298 agreement between the methods.

299
300 Six studies used a leg to leg technology for assessing FM, albeit Loenneke et al. (Loenneke et al. 2013) utilized two
301 different predictive equations, as reported in Table 1, for a total of seven comparisons. Three of them reported an
302 underestimation in %FM (Civar et al. 2003; Loenneke et al. 2013) and FM (Dixon et al. 2005), two studies an
303 overestimation in FM (Domingos et al. 2019; Graybeal et al. 2020), while three studied showed no difference (Civar et
304 al. 2006; Loenneke et al. 2013; Graybeal et al. 2020). Considering the Graybeal et al. (Graybeal et al. 2020) study, higher
305 FM was found only in men, while no difference was reported for women. In the Loenneke et al. (Loenneke et al. 2013)
306 study, no difference was found when the device was set on the “non-athlete” mode, while FM was underestimated using
307 the “athletes” modality. Only Graybeal et al. (Graybeal et al. 2020) assessed FFM and reported a good agreement with
308 the reference method for women and an underestimation for men. No study involving leg to leg BIA-technologies reported
309 the predictive equations used.

310
311
312
313
314
315
316
317
318
319
320
321
322
323
324
325
326
327
328
329
330
331
332
333
334
335
336
337
338
339
340
341
342
343
344
345
346
347
348
349
350
351
352
353
354
355
356
357
358
359
360
361
362
363
364
365

310
1
311
2
3
312
4
5
313
6
7
314
8
9
315
10
11
316
12
13
317
14
15
318
16
17
319
18
19
320
20
21
321
22
23
322
24
25
323
26
27
324
28
29
325
30
31
326
32
33
327
34
35
328
36
37
329
38
39
330
40
41
331
42
43
332
44
45
333
46
47
334
48
49
335
50
51
336
52
53
337
54
55
338
56
57
339
58
59
340
60
61
62
63
64
65

Four studies used a hand to hand technology and reported an underestimation in %FM (Esco et al. 2011; Loenneke et al. 2013; Graybeal et al. 2020; Syed-Abdul et al. 2021), albeit Loenneke et al. (Loenneke et al. 2013) and Syed-Abdul et al. (Syed-Abdul et al. 2021) utilized different predictive equations, as reported in Table 1, for a total of eight comparisons. Of these four studies, Loenneke et al. (Loenneke et al. 2013) and Syed-Abdul et al. (Syed-Abdul et al. 2021) reported lower %FM when the devices were set on the “athlete” modality, and a good agreement when the devices were set on the “non-athlete” modality. Graybeal et al. (Graybeal et al. 2020) overestimated %FM in men, while no difference for women was found; additionally, FFM was underestimated in men and a good agreement for women was found. No studies involving hand to hand BIA technologies reported the predictive equations used.

Insert Table 1 next here

BIA vs. reference methods: Body fluids estimations

Table 2 shows the study design, demographic information, bioimpedance methodology, reference methods, and the main results for each study. All seven studies assessing TBW were performed using the foot to hand technology, albeit different devices (Matias et al. 2016a) and procedures (Matias et al. 2016b; Deminice et al. 2016; Shiose et al. 2020; Coratella et al. 2021) for a total of 31 comparisons. Five studies reported no difference in TBW assessed by BIA vs. reference methods (Matias et al. 2016b, a; Shiose et al. 2020; Coratella et al. 2021; Francisco et al. 2021), four studies an underestimation (Matias et al. 2016a, b; Deminice et al. 2016; Coratella et al. 2021), and one study an overestimation (Matias et al. 2016a). Five studies used the foot to hand technology to assess ECW, albeit different devices (Matias et al. 2016a) and procedures (Matias et al. 2016a,b; Coratella et al. 2021) for a total of 12 comparisons. Five studies reported no difference in ECW assessed by BIA vs. reference methods (Birzniece et al. 2015; Matias et al. 2016a, b; Coratella et al. 2021; Francisco et al. 2021), four studies an underestimation (Birzniece et al. 2015; Matias et al. 2016a, b; Coratella et al. 2021), and no study reported an overestimation. Three studies (Matias et al. 2016a, b; Francisco et al. 2021) used the foot to hand technology to assess ICW, albeit different devices (Matias et al. 2016a) for a total of four comparisons. All comparisons showed no difference in ICW assessed by BIA vs. reference techniques. Only five out of these seven studies (Matias et al. 2016a, b; Deminice et al. 2016; Shiose et al. 2020; Coratella et al. 2021) reported the predictive equations used.

Insert Table 2 next here

341 BIVA vs. reference methods

1
342

3
343 Five studies compared the BIVA's outcomes with body composition measurements obtained from reference methods, as
5
344 shown in Table 3. All the analyzed studies were conducted using a foot to hand technology. Two studies were conducted
7
345 with a cross-sectional design (Marini et al. 2020; Stagi et al. 2021), and showed that the *specific* vector length was
9
346 correlated positively with %FM and the classic vector negatively with TBW, both at the whole body (Marini et al. 2020)
11
347 and the segmental level (Stagi et al. 2021). These findings were also confirmed in three longitudinal studies (Campa et
13
348 al. 2020, 2021a; Silva et al. 2020), which highlighted the effectiveness of BIVA in assessing changes in body composition
15
349 over time. In addition to the vector length evaluation, its position along the minor axis of the BIVA ellipses, that is mainly
17
350 due to phase angle variations, has been associated with the ICW/ECW ratio (Campa et al. 2020, 2021a; Marini et al. 2020;
19
351 Silva et al. 2020).

21
352

23
353

Insert Table 3 next here

25
354

27
355

Discussion

29
356

31
357

The present systematic review aimed to compare i) BIA vs. reference methods in the estimation of body composition
33
358 parameters in athletes and ii) BIVA vs. reference methods in the qualitative assessment of body composition parameters
35
359 in athletes. Forty-two studies were included in the review, for a total of 2978 athletes involved in team or individual
37
360 sports. Overall, most of the studies included used the foot to hand technology, allowing to draw a detailed picture of the
39
361 BIA or BIVA vs. reference methods for FM FFM and body fluids, quantitative and qualitative assessment, respectively.

41
362

The remaining hand to hand, leg to leg, and direct segmental technologies were used in few studies, and none of these
43
363 assessed body fluids, so that the comparison is incomplete.

45
364

47
365

BIA vs. reference methods: FM and FFM

49
366

The studies that assessed FM and FFM using BIA vs. reference methods resulted in inconsistent findings. Concerning the
51
367 FM, BIA showed poor accuracy vs. the reference methods, regardless of the technology used. However, while in some
53
368 studies the authors used a direct formula to determine %FM (Colville et al. 1989; Pichard et al. 1997), in other studies
55
369 FM was indirectly derived as the difference between the body mass and FFM (De Lorenzo et al. 2000; Houtkoop et al.
57
370 2001; Andreoli et al. 2004; Company and Ball 2010). In addition, although the same predictive equations were used
59
371 (Oppliger et al. 1991), different reference methods were chosen to determine %FM, such as 4C (Andreoli et al. 2004) or

61
62

63
64

65

372 DXA (De Lorenzo et al. 2000). However, a lack of agreement between 4C and DXA was later observed when assessing
373 %FM in athletes (Santos et al. 2010), making the comparison between BIA and the reference methods challenging. To
374 further entangle this picture, several studies that used the foot to hand (Kirkendall et al. 1991; Hortobágyi et al. 1992;
375 Williams and Bale 1998; Houtkoop et al. 2001; Svantesson et al. 2008; Birzniece et al. 2015; Krzykała et al. 2016; Arias
376 Téllez et al. 2019; Graybeal et al. 2020), and all the studies that used the hand to hand, the leg to leg and the direct
377 segmental technology, did not report the predictive equations used for determining %FM. Interestingly, two studies
378 (Loenneke et al. 2013; Syed-Abdul et al. 2021) that used hand to hand devices found no difference between BIA and the
379 reference methods when the device was set on the "non-athlete" mode, while an underestimation in %FM was observed
380 when the "athlete" mode was set. According to the manufacturer of the device used by Loenneke et al. (Loenneke et al.
381 2013), the "athletic" mode is utilized for individuals who have exercised at least 10 hours a week consistently for at least
382 6 months, or who have a resting heart rate of 60 bpm or less. These factors may not exclude that an athlete may have
383 different characteristics. In this regard, an actual definition of athlete is advocated, so to define clearly when a specific or
384 generalized equation or modality should be used.

385
386 Using the foot to hand technology coupled with predictive equations developed for athletes, BIA showed no difference
387 with reference methods for estimating FFM (Lukaski et al. 1990; Fornetti et al. 1999; Graybeal et al. 2020; Matias et al.
388 2021) and its LST component (Sardinha et al. 2020). On the contrary, when generalized equations were used, inconclusive
389 findings were observed. Regarding the direct segmental technology, BIA showed an underestimation of FFM compared
390 to the reference methods. Only one study assessed FFM using the leg to leg and hand to hand technology, reporting
391 underestimation in men and good agreement in women for both technologies (Graybeal et al. 2020). In conclusion, the
392 present state of the art needs to be implemented with procedures including the gold standard procedure for determining
393 %FM and FFM (4C) and predictive equations for athletes, reported in the protocol. Considering that the Matias et al.
394 (Matias et al. 2021) equation is the only one developed with 4C, its use should be preferred when assessing FFM in
395 athletes.

396 397 BIA vs. reference methods: body fluids estimations

398
399 All the studies comparing BIA vs. reference methods to assess body fluids were conducted using the foot to hand
400 technology and the dilution techniques as the reference method. Such a consistency allows more robust outcomes when
401 summarizing the results. Considering all the studies, the use of predictive equations for athletes (Matias et al. 2016b)
402 resulted in good agreement with the dilution techniques. Notably, the Matias' equations (Matias et al. 2016b) were

403 developed for the foot to hand technology at a 50 kHz frequency, and are to date the only available ones. In contrast, the
404 use of generalized predictive equations (Kushner and Schoeller 1986; Van Loan and Mayclin 1987; Lukaski and
405 Bolonchuk 1988; Kushner et al. 1992; Sergi et al. 1994; Schoeller and Luke 2000; Morgenstern et al. 2002; Sun et al.
406 2003) led to an overall underestimation of the body fluids. Lastly, BIA was also shown to be a valid method for assessing
407 body fluids in person with varying hydration status (Francisco et al. 2021).

408

409 BIVA vs. reference methods.

410 BIVA is an alternative method to qualitatively assess body composition in athletes. It allows the analysis of the
411 ICW/ECW ratio and the amount of TBW (Classic BIVA) or %FM (Specific BIVA) (Campa et al. 2021b). Since these
412 techniques are based on raw data, BIVA does not require the use of predictive equations, avoiding possible errors due to
413 their improper application. On the other hand, BIVA does not provide estimates of volume or mass, but a classification
414 (e.g., more or less body fluids or %FM) and ranking (e.g., better or worse after treatment or intervention) tool (Lukaski
415 and Raymond-Pope 2021). In this regard, a rightward or leftward displacement of the BIVA vector is interpreted as a
416 decrease or increase in the ICW/ECW ratio, respectively; moreover, longer vectors corresponds to lower TBW (Classic
417 BIVA) or higher %FM (*Specific BIVA*) and vice versa (Campa et al. 2021b). All the selected studies agree in suggesting
418 BIVA as a valid method for assessing body composition in athletes compared to the reference methods. Specifically, the
419 standard reference methods were 4C (Marini et al. 2020), dilution techniques (Marini et al. 2020; Campa et al. 2020; Silva
420 et al. 2020) and DXA (Marini et al. 2020; Stagi et al. 2021; Campa et al. 2021a). Notably, BIVA was derived from the
421 foot to hand technology only. This leads to some considerations. In first instance, the reference tolerance ellipses for
422 athletes have been designed for the foot to hand technology, so that different technology should not be used due to the
423 lack of agreement between the technologies (Silva et al. 2019; Dellinger et al. 2021; Stratton et al. 2021). Secondly, when
424 the aim of the research is to compare an athlete with his peers, the tolerance ellipses have been designed for some athletic
425 populations, such as soccer (Micheli et al. 2014; Bongiovanni et al. 2020), volleyball (Campa and Toselli 2018), cycling
426 (Giorgi et al. 2018), or endurance, sports team or power/velocity (Campa et al. 2019) athletes. All other sports should be
427 redirected to the tolerance ellipses for generic athletic population (Campa et al. 2019).

428

429 Limitations of the review and future perspectives

430 A few limitations to this review should be acknowledged. Firstly, we classified the results according to the BIA
431 technology used in the selected studies. However, even within the same technology, there could be confounding factors.
432 For example, the positioning of the electrodes used in the foot to hand technologies and their typology could lead to
433 different outcomes, increasing the variability within the results. In this regard, recent guidelines have been proposed to

434
435
436
437
438
439
440
441
442
443
444
445
446
447
448
449
450
451
452
453
454
455
456
457
458
459
460
461
462
463
464
465

434 avoid inconsistent procedures (Campa et al. 2021b). Secondly, several devices have been considered, which could have
1
435 different characteristics that may represent a further confounding factor, such as the amperage and their reliability.
2
3
436 Furthermore, regardless of the BIA-devices and technologies used, the athlete's evaluation must consider numerous
4
5
437 factors such as the hours since last exercise and the nutrition prior to the test (Lukaski et al. 1990). A number of future
6
7
438 perspectives also arise from these results. For example, future longitudinal studies are warranted, assessing the
8
9
439 responsiveness of different BIA technologies in comparison with the reference methods. Moreover, further studies are
10
11
440 needed to understand which factors (e.g., amperage, body segments measured, experimental conditions) other than
12
13
441 technologies increase the between-device variability. Lastly, authors are encouraged to provide raw bioelectrical data to
14
15
442 a more transparent assessment of body composition through BIA and BIVA.
16
17

18
19

20 **Conclusions**

21
22
23
24
25
26
27
28
29
30
31
32
33
34
35
36
37
38
39
40
41
42
43
44
45
46
47
48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65

Regardless of the BIA-technology, the assessment of FM% results in lack of agreement with the reference methods. When estimating FFM using predictive equations developed for athletes and the foot to hand technology, a good agreement with the reference methods has been observed. Generalized equations lead to an underestimation of FFM. Similarly, body fluids are accurately estimated using predictive equations for athletes and the foot to hand technology, while overall underestimated using generalized equations. Regarding BIVA, Classic and *Specific* approaches represented two valid methods for assessing body fluids (Classic BIVA) and percentage of fat mass (*Specific* BIVA). The present systematic review suggests that BIA and BIVA could be used for assessing body composition in athletes, provided that equations and BIVA references developed for athletes are used. Figure 4 summarizes the main finding of the present systematic review.

Insert Figure 4 next here

66 **References**

- 67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95
96
97
98
99
100
- Andreoli A, Melchiorri G, Volpe SL, et al (2004) Multicompartment model to assess body composition in professional water polo players. *J Sports Med Phys Fitness* 44:38–43
- Arias Téllez MJ, Carrasco F, España Romero V, et al (2019) A comparison of body composition assessment methods in climbers: Which is better? *PLoS One* 14:e0224291. <https://doi.org/10.1371/journal.pone.0224291>
- Birzniece V, Khaw C-H, Nelson AE, et al (2015) A critical evaluation of bioimpedance spectroscopy analysis in estimating body composition during GH treatment: comparison with bromide dilution and dual X-ray absorptiometry. *Eur J Endocrinol* 172:21–28. <https://doi.org/10.1530/EJE-14-0660>

- 465 Boileau RA, Horswill CA (2000) Body composition in sports: Measurement and applications for weight gain and loss.
466 In: Garret Jr WE, Kinkendall DT (eds) Exercise and Sport Science. Lippincott Williams & Wilkins, Philadelphia:
467 Saunders, pp 319–338
- 468 Bongiovanni T, Mascherini G, Genovesi F, et al (2020) Bioimpedance Vector References Need to Be Period-Specific
469 for Assessing Body Composition and Cellular Health in Elite Soccer Players: A Brief Report. *J Funct Morphol*
470 *Kinesiol* 5: <https://doi.org/10.3390/jfmk5040073>
- 471 Brewer GJ, Blue MNM, Hirsch KR, et al (2019) Appendicular Body Composition Analysis: Validity of Bioelectrical
472 Impedance Analysis Compared With Dual-Energy X-Ray Absorptiometry in Division I College Athletes. *J*
473 *strength Cond Res* 33:2920–2925. <https://doi.org/10.1519/JSC.0000000000003374>
- 474 Buffa R, Saragat B, Cabras S, et al (2013) Accuracy of specific BIVA for the assessment of body composition in the
475 United States population. *PLoS One* 8:e58533. <https://doi.org/10.1371/journal.pone.0058533>
- 476 Campa F, Matias C, Gatterer H, et al (2019) Classic Bioelectrical Impedance Vector Reference Values for Assessing
477 Body Composition in Male and Female Athletes. *Int J Environ Res Public Health* 16:
478 <https://doi.org/10.3390/ijerph16245066>
- 479 Campa F, Matias CN, Marini E, et al (2020) Identifying athlete body fluid changes during a competitive season with
480 bioelectrical impedance vector analysis. *Int J Sports Physiol Perform* 15:361–367.
481 <https://doi.org/10.1123/ijsp.2019-0285>
- 482 Campa F, Matias CN, Nunes CL, et al (2021a) Specific Bioelectrical Impedance Vector Analysis Identifies Body Fat
483 Reduction after a Lifestyle Intervention in Former Elite Athletes. *Biology (Basel)*
484 10:<https://doi.org/10.3390/biology10060524>
- 485 Campa F, Toselli S (2018) Bioimpedance Vector Analysis of Elite, Sub-Elite and Low-Level Male Volleyball Players.
486 *Int J Sports Physiol Perform* 1–13. <https://doi.org/10.1123/ijsp.2018-0039>
- 487 Campa F, Toselli S, Mazzilli M, et al (2021b) Assessment of Body Composition in Athletes: A Narrative Review of
488 Available Methods with Special Reference to Quantitative and Qualitative Bioimpedance Analysis. *Nutrients* 13:
489 <https://doi.org/10.3390/nu13051620>
- 490 Castizo-Olier J, Iruiria A, Jemni M, et al (2018) Bioelectrical impedance vector analysis (BIVA) in sport and exercise:
491 Systematic review and future perspectives. *PLoS One* 13:e0197957. <https://doi.org/10.1371/journal.pone.0197957>
- 492 Civar S, Aktop A, Tercan E, et al (2006) Validity of leg-to-leg bioelectrical impedance measurement in highly active
493 women. *J strength Cond Res* 20:359–365. <https://doi.org/10.1519/R-15884.1>
- 494 Civar S, Ozer M, Aktop A, et al (2003) Validity of leg-to-leg bioelectrical impedance measurement in highly active
495 males. *Biol Sport* 20:

- 496 Colville B, Heyward V, Sandoval W (1989) Comparison of Two Methods for Estimating Body Composition of
1
497 Bodybuilders. *J Strength Cond Res* 3:5W_61
2
3
498 Company J, Ball S (2010) Body Composition Comparison: Bioelectric Impedance Analysis with Dual-Energy X-Ray
4
5
499 Absorptiometry in Adult Athletes. *Meas Phys Educ Exerc Sci* 14:186–201.
6
7
500 <https://doi.org/10.1080/1091367X.2010.497449>
8
9
501 Coratella G, Campa F, Matias CN, et al (2021) Generalized bioelectric impedance-based equations underestimate body
10
502 fluids in athletes. *Scand J Med Sci Sports*. <https://doi.org/10.1111/sms.14033>
11
12
503 De Lorenzo A, Andreoli A, Matthie J, Withers P (1997) Predicting body cell mass with bioimpedance by using
13
14
504 theoretical methods: a technological review. *J Appl Physiol* 82:1542–1558.
15
16
505 <https://doi.org/10.1152/jappl.1997.82.5.1542>
17
18
506 De Lorenzo A, Bertini I, Iacopino L, et al (2000) Body composition measurement in highly trained male athletes. A
19
20
507 comparison of three methods. *J Sports Med Phys Fitness* 40:178–183
21
22
508 Dellinger JR, Johnson BA, Benavides ML, et al (2021) Agreement of bioelectrical resistance, reactance, and phase
23
24
509 angle values from supine and standing bioimpedance analyzers. *Physiol Meas*
25
26
510 Deminice R, Rosa FT, Pfrimer K, et al (2016) Creatine Supplementation Increases Total Body Water in Soccer Players:
27
28
511 a Deuterium Oxide Dilution Study. *Int J Sports Med* 37:149–153. <https://doi.org/10.1055/s-0035-1559690>
29
30
512 Deurenberg P, Kusters CS, Smit HE (1990) Assessment of body composition by bioelectrical impedance in children
31
32
513 and young adults is strongly age-dependent. *Eur J Clin Nutr* 44:261–268
33
34
514 Deurenberg P, van der Kooy K, Leenen R, et al (1991) Sex and age specific prediction formulas for estimating body
35
36
515 composition from bioelectrical impedance: a cross-validation study. *Int J Obes* 15:17–25
37
38
516 Dixon CB, Deitrick RW, Pierce JR, et al (2005) Evaluation of the BOD POD and leg-to-leg bioelectrical impedance
39
40
517 analysis for estimating percent body fat in National Collegiate Athletic Association Division III collegiate
41
42
518 wrestlers. *J strength Cond Res* 19:85–91. <https://doi.org/10.1519/14053.1>
43
44
519 Domingos C, Matias CN, Cyrino ES, et al (2019) The usefulness of Tanita TBF-310 for body composition assessment
45
46
520 in Judo athletes using a four-compartment molecular model as the reference method. *Rev Assoc Med Bras*
47
48
521 65:1283–1289. <https://doi.org/10.1590/1806-9282.65.10.1283>
49
50
522 Esco M, Olson MS, Williford H, et al (2011) The Accuracy of Hand-to-Hand Bioelectrical Impedance Analysis in
51
52
523 Predicting Body Composition in College-Age Female Athletes. *J Strength Cond Res* 25:1040–1045
53
54
524 Esco MR, Snarr RL, Leatherwood MD, et al (2015) Comparison of total and segmental body composition using DXA
55
56
525 and multifrequency bioimpedance in collegiate female athletes. *J strength Cond Res* 29:918–925.
57
58
526 <https://doi.org/10.1519/JSC.0000000000000732>
59
60
61
62
63
64
65

- 527 Fornetti WC, Pivarnik JM, Foley JM, Fiechtner JJ (1999) Reliability and validity of body composition measures in
1 female athletes. *J Appl Physiol* 87:1114–1122. <https://doi.org/10.1152/jappl.1999.87.3.1114>
28
- 3
529 Francisco R, Jesus F, Gomes T, et al (2021) Validity of water compartments estimated using bioimpedance
5 spectroscopy in athletes differing in hydration status. *Scand J Med Sci Sports* 31:1612–1620.
6
7
531 <https://doi.org/10.1111/sms.13966>
9
- 532 Giorgi A, Vicini M, Pollastri L, et al (2018) Bioimpedance patterns and bioelectrical impedance vector analysis (BIVA)
11 of road cyclists. *J Sports Sci* 1–6. <https://doi.org/10.1080/02640414.2018.1470597>
13
- 534 Graves JE, Pollock ML, Colvin AB, et al (1989) Comparison of different bioelectrical impedance analyzers in the
15 prediction of body composition. *Am J Hum Biol Off J Hum Biol Counc* 1:603–611.
535
17
536 <https://doi.org/10.1002/ajhb.1310010511>
19
- 537 Graybeal AJ, Moore ML, Cruz MR, Tinsley GM (2020) Body Composition Assessment in Male and Female
21 Bodybuilders: A 4-Compartment Model Comparison of Dual-Energy X-Ray Absorptiometry and Impedance-
538 Based Devices. *J strength Cond Res* 34:1676–1689. <https://doi.org/10.1519/JSC.0000000000002831>
23
- 539 Hannan WJ, Cowen SJ, Freeman CP, Wrate RM (1993) Can bioelectrical impedance improve the prediction of body fat
25 in patients with eating disorders? *Eur J Clin Nutr* 47:741–746
540
27
541
29
- 542 Hartmann Nunes RF, de Souza Bezerra E, Orssatto LB, et al (2020) Assessing body composition in rugby players:
31 agreement between different methods and association with physical performance. *J Sports Med Phys Fitness*
543 60:733–742. <https://doi.org/10.23736/S0022-4707.20.10487-0>
33
- 544
35
- 545 Heitmann BL (1990) Evaluation of body fat estimated from body mass index, skinfolds and impedance. A comparative
37 study. *Eur J Clin Nutr* 44:831–837
546
39
- 547 Heymsfield S, Lohman T, Wang Z, Going S (2005) Human body composition, 2nd edn. Human Kinetics, Leeds in
41 Champaign, IL
548
43
- 549 Hortobágyi T, Israel RG, Houmard JA, et al (1992) Comparison of four methods to assess body composition in black
45 and white athletes. *Int J Sport Nutr* 2:60–74. <https://doi.org/10.1123/ijnsn.2.1.60>
550
47
- 551 Houtkoop L, Mullins VA, Going SB, et al (2001) Body composition profiles of elite American heptathletes. *Int J Sport*
49 *Nutr Exerc Metab* 11:162–173. <https://doi.org/10.1123/ijnsnem.11.2.162>
50
- 552
51
- 553 Kirkendall DT, Grogan JW, Bowers RG (1991) Field comparison of body composition techniques: hydrostatic
53 weighing, skinfold thickness, and bioelectric impedance. *J Orthop Sports Phys Ther* 13:235–239.
54
55
554
55
555
56
556
57
- 557 Kotler DP, Burastero S, Wang J, Pierson Jr RN (1996) Prediction of body cell mass, fat-free mass, and total body water
60 with bioelectrical impedance analysis: effects of race, sex, and disease. *Am J Clin Nutr* 64:489S–497S.
61
62
63
64
65

- 558 <https://doi.org/10.1093/ajcn/64.3.489S>
- 1
559 Krzykała M, Konarski JM, Malina RM, et al (2016) Fatness of female field hockey players: Comparison of estimates
3
560 with different methods. *Homo* 67:245–257. <https://doi.org/10.1016/j.jchb.2016.03.003>
- 5
561 Kushner R, Schoeller DA, Fjeld CR, Danford L (1992) Is the Impedance index (ht^2/R) significant in predicting total
7
562 body water? *Am J Clin Nutr* 56:835–839. <https://doi.org/10.1093/ajcn/56.5.835>
- 9
563 Kushner RF, Schoeller DA (1986) Estimation of total body water by bioelectrical impedance analysis. *Am J Clin Nutr*
11
564 44:417–424. <https://doi.org/10.1093/ajcn/44.3.417>
- 13
565 Kyle UG, Bosaeus I, De Lorenzo AD, et al (2004a) Bioelectrical impedance analysis--part I: review of principles and
15
566 methods. *Clin Nutr* 23:1226–1243. <https://doi.org/10.1016/j.clnu.2004.06.004>
- 17
567 Kyle UG, Bosaeus I, De Lorenzo AD, et al (2004b) Bioelectrical impedance analysis-part II: utilization in clinical
19
568 practice. *Clin Nutr* 23:1430–1453. <https://doi.org/10.1016/j.clnu.2004.09.012>
- 21
569 Lee L-C, Hsu P-S, Hsieh K-C, et al (2021) Standing 8-Electrode Bioelectrical Impedance Analysis as an Alternative
23
570 Method to Estimate Visceral Fat Area and Body Fat Mass in Athletes. *Int J Gen Med* 14:539–548.
25
571 <https://doi.org/10.2147/IJGM.S281418>
- 27
572 Loenneke JP, Wilson JM, Wray ME, et al (2012) The estimation of the fat free mass index in athletes. *Asian J Sports*
29
573 *Med* 3:200–203. <https://doi.org/10.5812/asjms.34691>
- 31
574 Loenneke JP, Wray ME, Wilson JM, et al (2013) Accuracy of field methods in assessing body fat in collegiate baseball
33
575 players. *Res Sports Med* 21:286–291. <https://doi.org/10.1080/15438627.2013.792087>
- 35
576 Lohman TG (1992) Advances in body composition assessment. *Cad. Saude Publica* 9:S116–S117
- 37
577 Lukaski H, Bolonchuk W (1987) Theory and validation of the tetrapolar bioelectrical impedance method to assess
39
578 human body composition
- 41
579 Lukaski H, Raymond-Pope CJ (2021) New Frontiers of Body Composition in Sport. *Int J Sports Med*.
43
580 <https://doi.org/10.1055/a-1373-5881>
- 45
581 Lukaski HC, Bolonchuk WW (1988) Estimation of body fluid volumes using tetrapolar bioelectrical impedance
47
582 measurements. *Aviat Space Environ Med* 59:1163–1169
- 48
49
50
583 Lukaski HC, Bolonchuk WW, Hall CB, Siders WA (1986) Validation of tetrapolar bioelectrical impedance method to
51
584 assess human body composition. *J Appl Physiol* 60:1327–1332. <https://doi.org/10.1152/jappl.1986.60.4.1327>
- 52
53
54
585 Lukaski HC, Bolonchuk WW, Siders WA, Hall CB (1990) Body composition assessment of athletes using bioelectrical
55
586 impedance measurements. *J Sports Med Phys Fitness* 30:434–440
- 56
57
58
587 Lukaski HC, Johnson PE, Bolonchuk WW, Lykken GI (1985) Assessment of fat-free mass using bioelectrical
59
60
61
588 impedance measurements of the human body. *Am J Clin Nutr* 41:810–817. <https://doi.org/10.1093/ajcn/41.4.810>
- 62
63
64
65

- 589 Lukaski HC, Piccoli A (2012) Bioelectrical impedance vector analysis for assessment of hydration in physiological
590 states and clinical conditions. In: Preedy V (ed) Handbook of Anthropometry. Springer, London, pp 287–305
- 591 Marini E, Campa F, Buffa R, et al (2020) Phase angle and bioelectrical impedance vector analysis in the evaluation of
592 body composition in athletes. *Clin Nutr* 39:447–454. <https://doi.org/10.1016/j.clnu.2019.02.016>
- 593 Matias CN, Campa F, Santos DA, et al (2021) Fat-free Mass Bioelectrical Impedance Analysis Predictive Equation for
594 Athletes using a 4-Compartment Model. *Int J Sports Med* 42:27–32. <https://doi.org/10.1055/a-1179-6236>
- 595 Matias CN, Júdeice PB, Santos DA, et al (2016a) Suitability of Bioelectrical Based Methods to Assess Water
596 Compartments in Recreational and Elite Athletes. *J Am Coll Nutr* 35:413–421.
597 <https://doi.org/10.1080/07315724.2015.1058198>
- 598 Matias CN, Santos DA, Júdeice PB, et al (2016b) Estimation of total body water and extracellular water with
599 bioimpedance in athletes: A need for athlete-specific prediction models. *Clin Nutr* 35:468–474.
600 <https://doi.org/10.1016/j.clnu.2015.03.013>
- 601 Micheli ML, Pagani L, Marella M, et al (2014) Bioimpedance and impedance vector patterns as predictors of league
602 level in male soccer players. *Int J Sports Physiol Perform* 9:532–539. <https://doi.org/10.1123/ijsp.2013-0119>
- 603 Moissl UM, Wabel P, Chamney PW, et al (2006) Body fluid volume determination via body composition spectroscopy
604 in health and disease. *Physiol Meas* 27:921–933. <https://doi.org/10.1088/0967-3334/27/9/012>
- 605 Morgenstern BZ, Mahoney DW, Warady BA (2002) Estimating total body water in children on the basis of height and
606 weight: a reevaluation of the formulas of Mellits and Cheek. *J Am Soc Nephrol* 13:1884–1888.
607 <https://doi.org/10.1097/01.asn.0000019920.30041.95>
- 608 NIH (2014) National Institution of Health: U. S Department of Health and Human Services. Quality assessment tool for
609 observational cohort and cross- sectional studies
- 610 Oppliger RA, Nielsen D, Hoegh J, Vance C (1991) Bioelectrical impedance prediction of fat free mass for high school
611 wrestlers validated. *Med Sci Sports Exerc* 23:S73
- 612 Page MJ, McKenzie JE, Bossuyt PM, et al (2021) The PRISMA 2020 statement: an updated guideline for reporting
613 systematic reviews. *BMJ* 372:n71. <https://doi.org/10.1136/bmj.n71>
- 614 Piccoli A, Rossi B, Pillon L, Bucciante G (1994) A new method for monitoring body fluid variation by bioimpedance
615 analysis: the RXc graph. *Kidney Int* 46:534–539
- 616 Pichard C, Kyle UG, Gremion G, et al (1997) Body composition by x-ray absorptiometry and bioelectrical impedance
617 in female runners. *Med Sci Sports Exerc* 29:1527–1534. <https://doi.org/10.1097/00005768-199711000-00021>
- 618 Raymond CJ, Dengel DR, Bosch TA (2018) Total and Segmental Body Composition Examination in Collegiate
619 Football Players Using Multifrequency Bioelectrical Impedance Analysis and Dual X-ray Absorptiometry. *J*

- 620 strength *Cond Res* 32:772–782. <https://doi.org/10.1519/JSC.0000000000002320>
- 621 Santos DA, Silva AM, Matias CN, et al (2010) Accuracy of DXA in estimating body composition changes in elite
622 athletes using a four compartment model as the reference method. *Nutr Metab (Lond)* 7:22.
623 <https://doi.org/10.1186/1743-7075-7-22>
- 624 Sardinha LB, Correia IR, Magalhães JP, et al (2020) Development and validation of BIA prediction equations of upper
625 and lower limb lean soft tissue in athletes. *Eur J Clin Nutr* 74:1646–1652. <https://doi.org/10.1038/s41430-020-0666-8>
- 626
- 627 Schoeller DA, Luke A (2000) Bioelectrical impedance analysis prediction equations differ between African Americans
628 and Caucasians, but it is not clear why. *Ann N Y Acad Sci* 904:225–226. <https://doi.org/10.1111/j.1749-6632.2000.tb06456.x>
- 629
- 630 Segal KR, Van Loan M, Fitzgerald PI, et al (1988) Lean body mass estimation by bioelectrical impedance analysis: a
631 four-site cross-validation study. *Am J Clin Nutr* 47:7–14. <https://doi.org/10.1093/ajcn/47.1.7>
- 632
- 633 Sergi G, Bussolotto M, Perini P, et al (1994) Accuracy of bioelectrical impedance analysis in estimation of extracellular
634 space in healthy subjects and in fluid retention states. *Ann Nutr Metab* 38:158–165.
635 <https://doi.org/10.1159/000177806>
- 636
- 637 Shiose K, Kondo E, Takae R, et al (2020) Validity of Bioimpedance Spectroscopy in the Assessment of Total Body
638 Water and Body Composition in Wrestlers and Untrained Subjects. *Int J Environ Res Public Health* 17:
639 <https://doi.org/10.3390/ijerph17249433>
- 640
- 641 Silva AM, Matias CN, Nunes CL, et al (2019) Lack of agreement of in vivo raw bioimpedance measurements obtained
642 from two single and multi-frequency bioelectrical impedance devices. *Eur J Clin Nutr* 73:1077–1083.
643 <https://doi.org/10.1038/s41430-018-0355-z>
- 644
- 645 Silva AM, Nunes CL, Matias CN, et al (2020) Usefulness of raw bioelectrical impedance parameters in tracking fluid
646 shifts in judo athletes. *Eur J Sport Sci* 20:734–743. <https://doi.org/10.1080/17461391.2019.1668481>
- 647
- 648 Stagi S, Irurtia A, Rosales Rafel J, et al (2021) Segmental body composition estimated by specific BIVA and dual-
649 energy X-ray absorptiometry. *Clin Nutr* 40:1621–1627. <https://doi.org/10.1016/j.clnu.2021.02.043>
- 650
- 651 Stahn A, Terblanche E, Gunga H-C (2012) Use of Bioelectrical Impedance: General Principles and Overview. In:
652 Preedy VR (ed) *Handbook of Anthropometry: Physical Measures of Human Form in Health and Disease*.
653 Springer New York, New York, NY, pp 49–90
- 654
- 655 Stolarczyk LM, Heyward VH, Hicks VL, Baumgartner RN (1994) Predictive accuracy of bioelectrical impedance in
656 estimating body composition of Native American women. *Am J Clin Nutr* 59:964–970.
657 <https://doi.org/10.1093/ajcn/59.5.964>
- 658
- 659
- 660
- 661
- 662
- 663
- 664
- 665

651 Stratton MT, Smith RW, Harty PS, et al (2021) Longitudinal agreement of four bioimpedance analyzers for detecting
652 changes in raw bioimpedance during purposeful weight gain with resistance training. *Eur J Clin Nutr* 75:1060–
653 1068. <https://doi.org/10.1038/s41430-020-00811-3>
654 Sun SS, Chumlea WC, Heymsfield SB, et al (2003) Development of bioelectrical impedance analysis prediction
655 equations for body composition with the use of a multicomponent model for use in epidemiologic surveys. *Am J*
656 *Clin Nutr* 77:331–340. <https://doi.org/10.1093/ajcn/77.2.331>
657 Svantesson U, Zander M, Klingberg S, Slinde F (2008) Body composition in male elite athletes, comparison of
658 bioelectrical impedance spectroscopy with dual energy X-ray absorptiometry. *J Negat Results Biomed* 7:1.
659 <https://doi.org/10.1186/1477-5751-7-1>
660 Syed-Abdul MM, Soni DS, Barnes JT, Waggener JD (2021) Comparative analysis of BIA, IBC and DXA for
661 determining body fat in American Football players. *J Sports Med Phys Fitness* 61:687–692.
662 <https://doi.org/10.23736/S0022-4707.21.11278-2>
663 Van Loan M, Mayclin P (1987) Bioelectrical Impedance Analysis: Is It a Reliable Estimator of Lean Body Mass and
664 Total Body Water? *Hum Biol* 69:299–309
665 Williams CA, Bale P (1998) Bias and limits of agreement between hydrodensitometry, bioelectrical impedance and
666 skinfold calipers measures of percentage body fat. *Eur J Appl Physiol Occup Physiol* 77:271–277.
667 <https://doi.org/10.1007/s004210050332>

668
669
670
671
672
673
674

Figure captions

Figure 1. Key concepts of bioelectrical impedance analysis.



Figure 2. PRISMA Flow chart of the studies' selection.

Figure 3. Bioelectrical devices and technologies involved in the selected studies.

Figure 4. Bioelectrical impedance analysis (BIA) vs. reference methods in athletes.

674
675

48
49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65

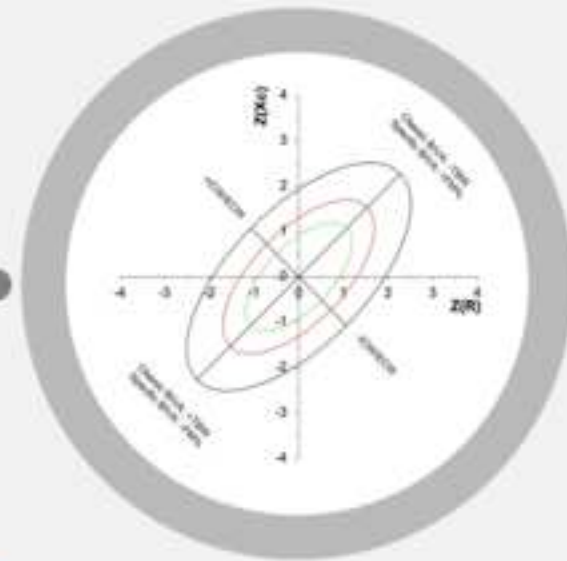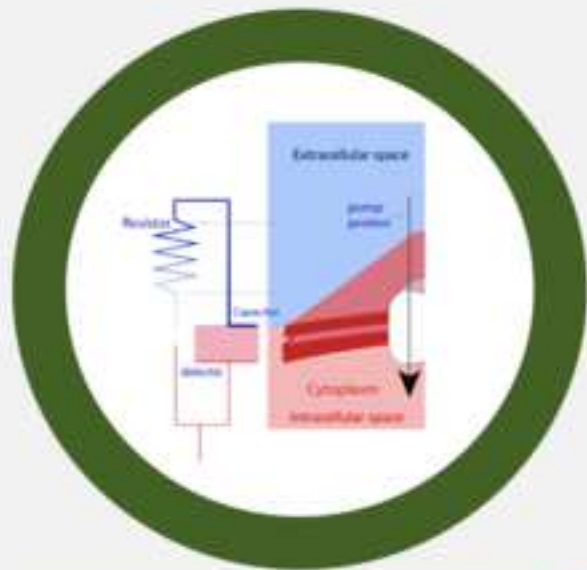

What does BIA measure?


- Impedance
- Resistance (R)
- Reactance (X_c)


How can BIA values be used?

- Insert it into predictive equations to estimate body composition
- Directly evaluated by bioelectrical impedance vector analysis (BIVA)

What does BIA provide?

- Quantification of body composition parameters
- Bivariate interpretation of R and X_c against the reference population percentiles

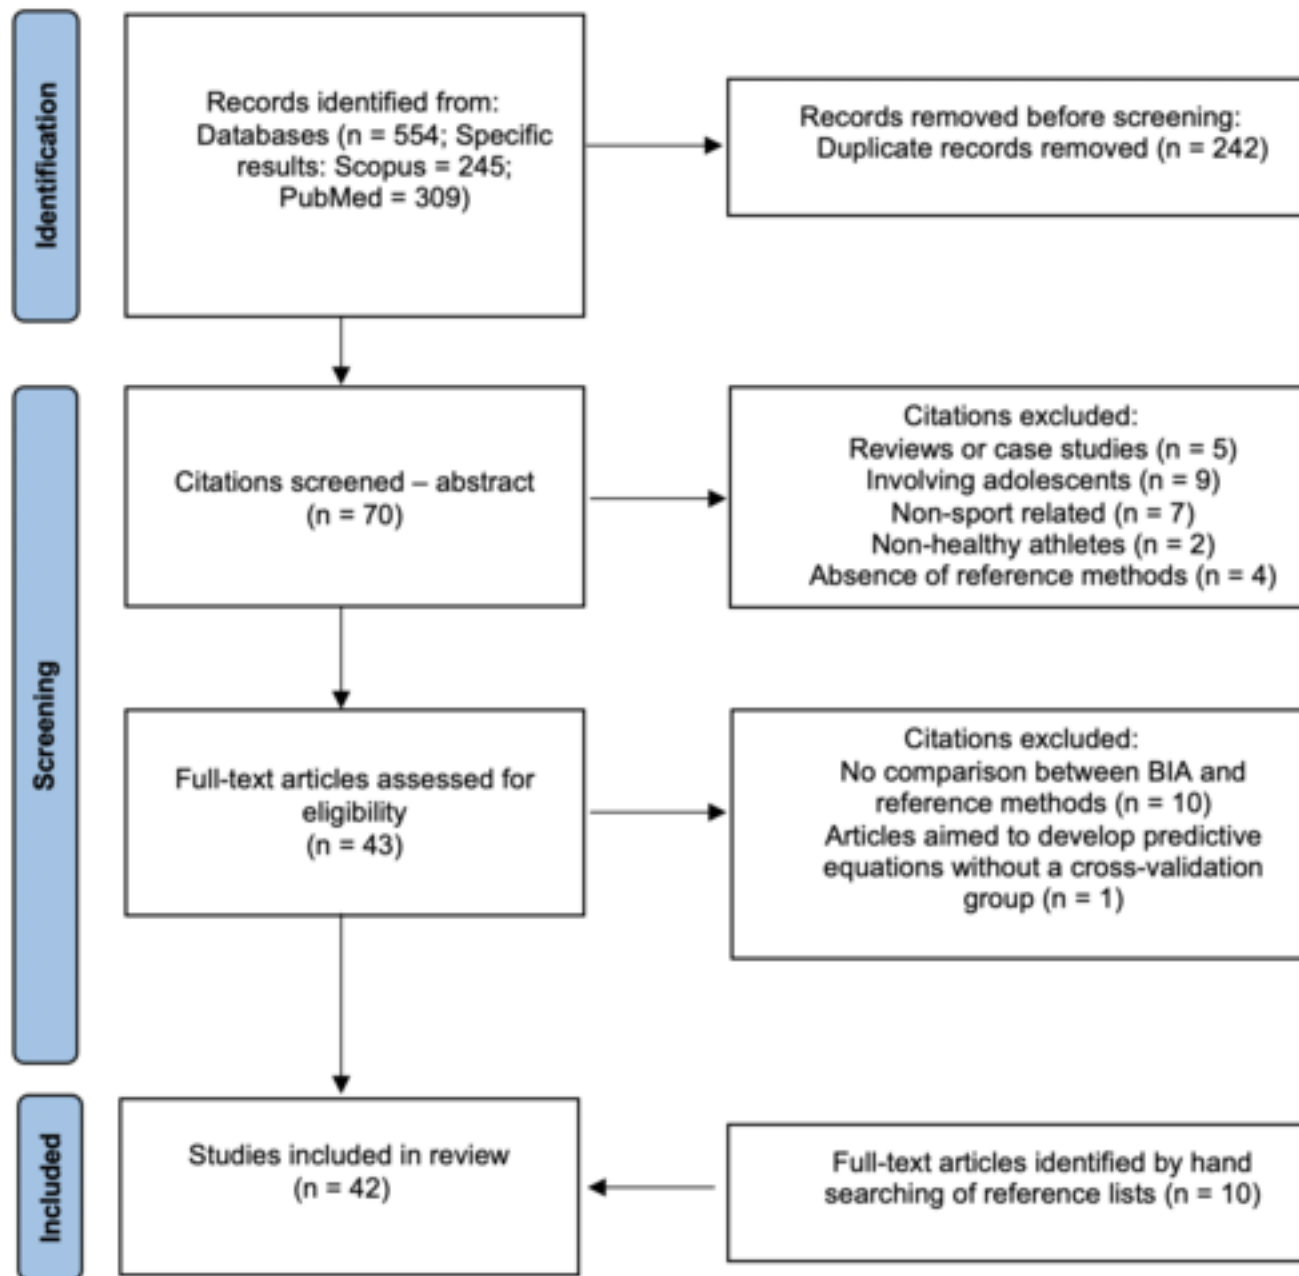

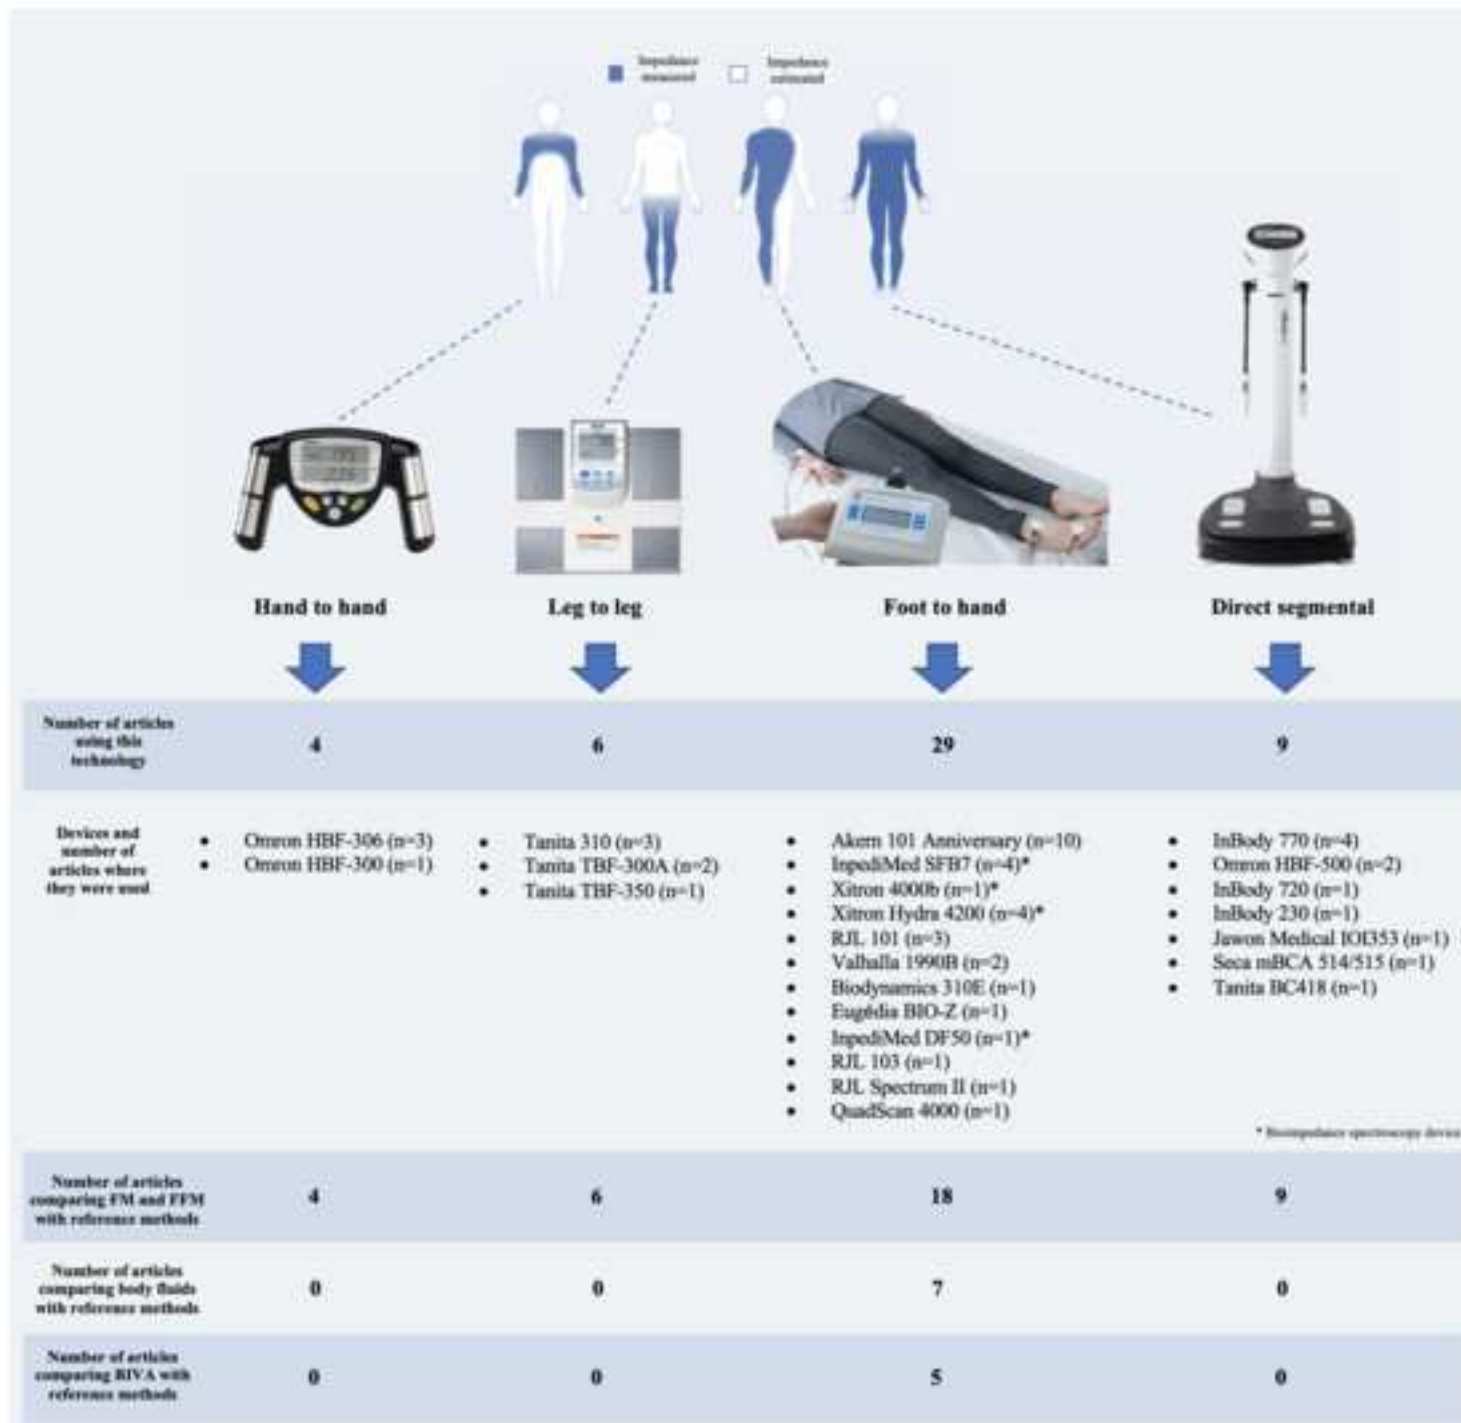

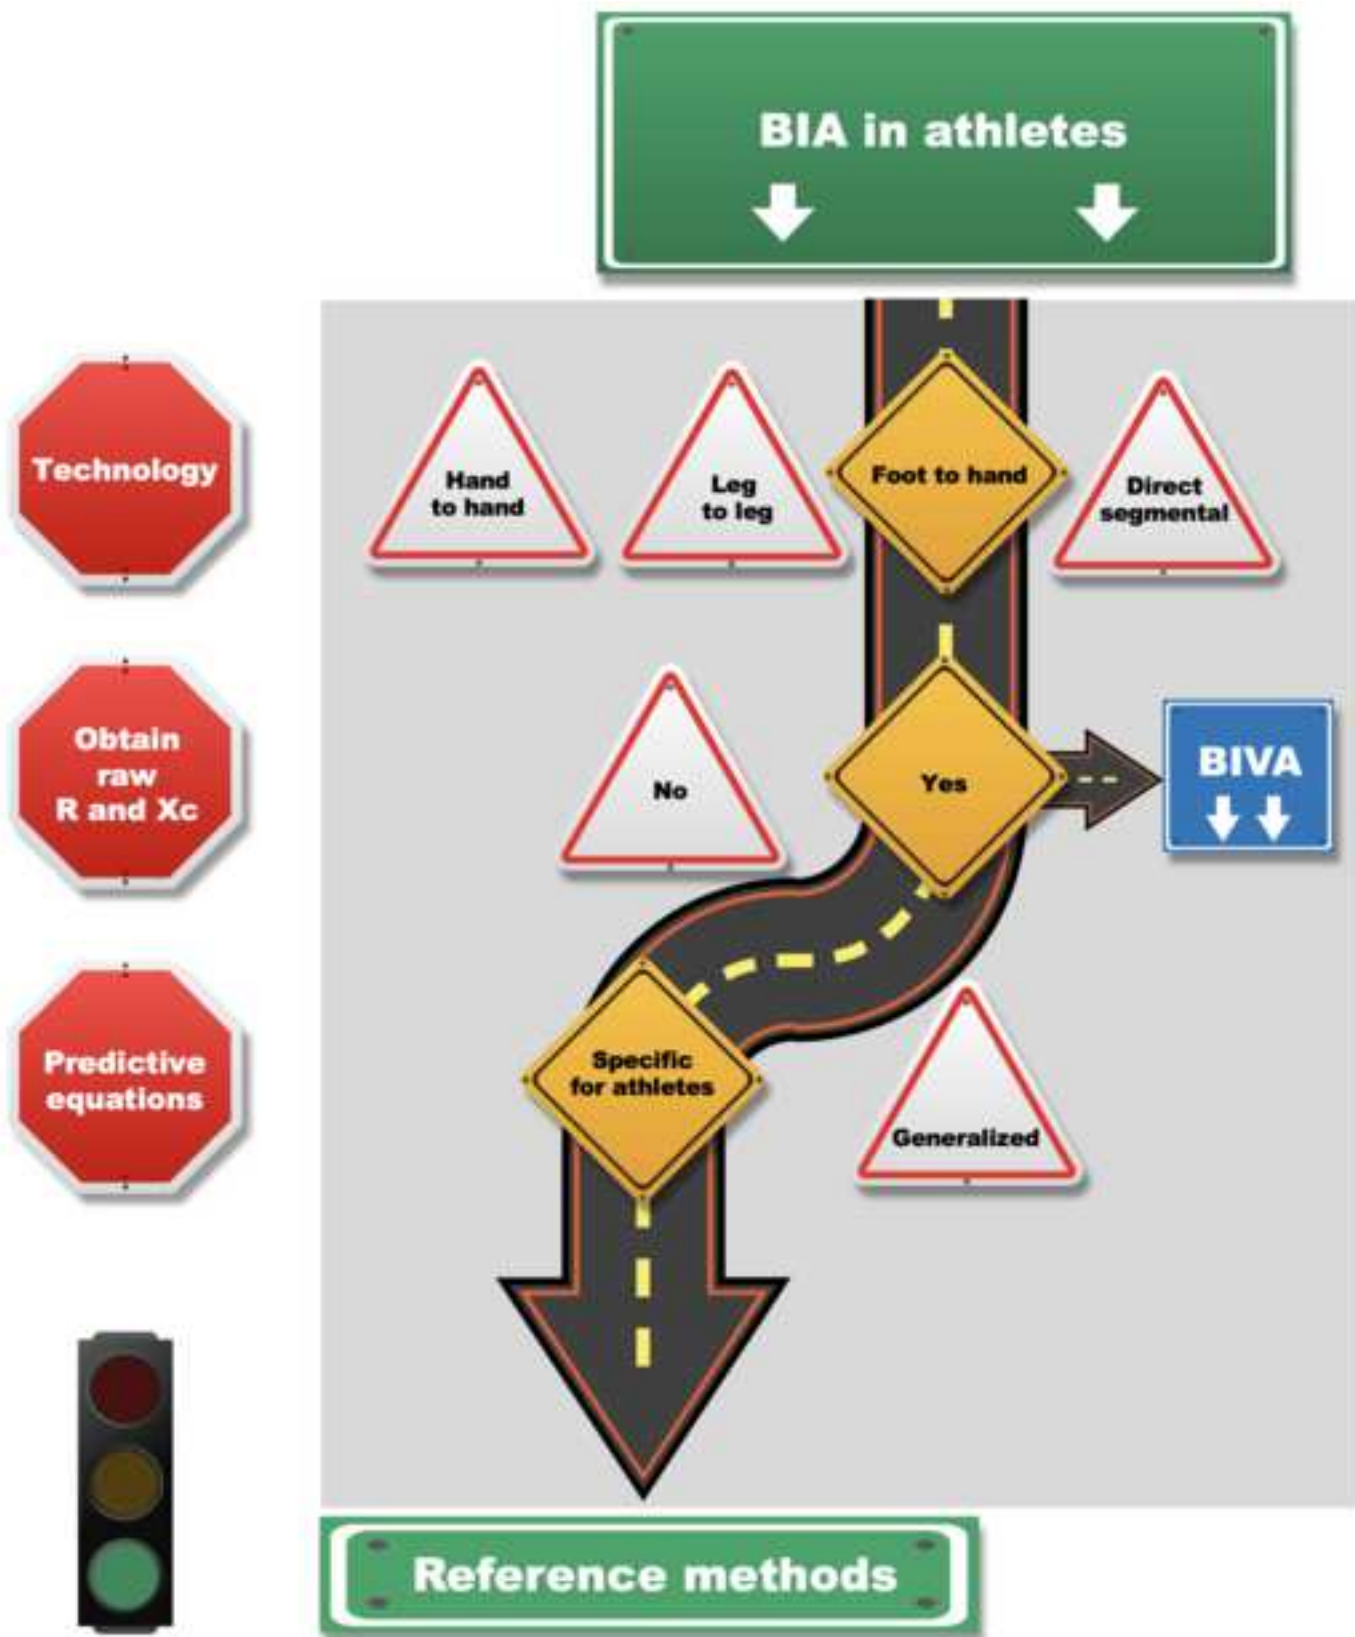


Table 1. Articles comparing bioimpedance outcomes with fat and fat-free mass and lean soft tissue derived using a reference method.

| Authors | Study design | Participants | Bioimpedance device / method | Sampling frequency (kHz) / Current (μA) | Analytical procedure | Reference method | Main results |
|--------------------------|-----------------|---|--|---|---|----------------------|---|
| (Colville et al. 1989) | Cross-sectional | 21 bodybuilders (men: n = 9, age 27.8 ± 5.7 y and women: n = 12, age 28.7 ± 7.2 y) | 103, RJL Systems, Detroit, MI / BIA using a foot to hand technology at single frequency | 50 / 800 | RJL Systems equation for men: %FM = [(Wt – FFM)/Wt] * 100, with FFM = 1.1554 – 0.0841*(Wt*R)/ S ² and for women: %FM = [(Wt – FFM)/Wt] * 100, with FFM = 1.113 – 0.00556*(Wt*R)/S ² | Hydrostatic weighing | BIA overestimated %FM (difference mean value: 7.5 %) and underestimated FFM (difference mean value: -4.8) in athletes considered as an entire group |
| (Lukaski et al. 1990) | Cross-sectional | 104 athletes (men: n = 58, age 20.7 ± 0.3 y and women: n = 46, age 19.8 ± 0.2 y) involved in different sports and divided into controlled and uncontrolled condition groups | 101, RJL Systems, Detroit, MI / BIA using a foot to hand technology at single frequency | 50 / 800 | (Lukaski and Bolonchuk 1987): FFM = 0.734*S ² /R + 0.116*Wt + 0.096*Xc + 0.876*Sex – 4.03, where 0 if female and 1 if male FM = Wt – FFM | Hydrostatic weighing | BIA showed no difference for the FFM estimation in controlled (difference mean value: 0.2 kg) and uncontrolled condition groups (difference mean value: 2.2 kg) BIA underestimated %FM in controlled (difference mean value: 0.2 %) and uncontrolled condition groups (difference mean value: 3.0 %) |
| (Kirkendall et al. 1991) | Cross-sectional | 29 male football players (age 27.0 ± 2.6 y) | Valhalla 1990B, Valhalla, San Diego, CA/ BIA using a foot to hand technology at single frequency | 50 / 500 | Equations owned by manufacturer | Hydrostatic weighing | BIA overestimated %FM (difference mean value: 5.0 %) |
| (Hortobágyi et al. 1992) | Cross-sectional | 90 men American football players: 55 blacks (age 19.4 ± 1.2 y) and whites (age 19.7 ± 1.5 y) | Spectrum II System, RJL Systems, Detroit, MI / BIA using a foot to hand | 50 / 800 | Equations owned by manufactures | Hydrostatic weighing | BIA overestimated %FM (blacks: difference mean value: 5.4 %; whites: difference mean value: 3.2 %) and underestimated FFM (blacks: difference mean value: 5.0 kg; whites: difference mean value: 3.3 kg) |

technology at single frequency

| | | | | | | | |
|-----------------------|-----------------|--------------------------------------|---|----------|---|-----|--|
| (Pichard et al. 1997) | Cross-sectional | 17 female runners (age 26.5 ± 1.4 y) | BIO-Z, Eugédia, Paris, France / BIA using a foot to hand technology at single frequency | 50 / 800 | <p>RJL Systems: %FM = 1 - (0.3981*S²/R + 0.3068*Wt + 0.095299) *(S - 100) + 0.7414/Wt) *100</p> <p>RJL Systems: FFM = 5.091 + 0.6483*S²/R + 0.1699*Wt</p> <p>(Lukaski et al. 1985): FFM = 3.04 + 0.85*S²/R</p> <p>(Lukaski et al. 1986): FFM = 4.917 + 0.821*S²/R</p> <p>(Lukaski and Bolonchuk 1987): FFM = 0.734*S²/R + 0.116*Wt + 0.096*Xc + 0.876*Sex - 4.03, where 0 if female and 1 if male</p> <p>(Van Loan and Mayclin 1987): FFM = 17.7868 + 0.00098 (S²) + 0.3736*Wt - 0.0238* R - 4.2921*Sex - 0.1531*Age, where 0 if female and 1 if male</p> | DXA | <p>RJL Systems equation overestimated %FM (difference mean value: 3.1 %)</p> <p>RJL Systems equation underestimated FFM (difference mean value: -0.8 kg)</p> <p>Lukaski's equation (Lukaski et al. 1985) underestimated FFM (difference mean value: -2.4 kg)</p> <p>Lukaski et al. equation (Lukaski et al. 1986) underestimated FFM (difference mean value: -1.9 kg)</p> <p>Lukaski and Bolonchuk (Lukaski and Bolonchuk 1987) equation underestimated FFM (difference mean value: -1.9 kg)</p> <p>Van Loan and Mayclin (Van Loan and Mayclin 1987) equation underestimated FFM (difference mean value: -2.8)</p> <p>Segal et al. (Segal et al. 1988) equation underestimated FFM (difference mean value: -2.8 kg)</p> <p>Graves et al. (Graves et al. 1989) equation underestimated FFM (difference mean value: -1.8 kg)</p> <p>Heitmann's equation (Heitmann 1990) underestimated FFM (difference mean value: -2.0 kg)</p> <p>Deurenberg et al. (Deurenberg et al. 1991) equation underestimated FFM (difference mean value: -4.9 kg)</p> |
|-----------------------|-----------------|--------------------------------------|---|----------|---|-----|--|

(Segal et al. 1988): FFM =
 $10.4349 + 0.000646*(S^2) -$
 $0.01397*R + 0.42087*Wt$

(Graves et al. 1989): FFM =
 $5.49 + 0.475*S^2/R +$
 $0.295*Wt$

(Heitmann 1990): FFM =
total body water/0.72*100,
with TBW = 11.03 +
 $0.266*S^2/R + 0.186*Wt +$
 $4.702*Sex - 0.081*Age,$
where 0 if female and 1 if
male

(Deurenberg et al. 1991):
 $FFM = S^2/R*0.34 + 0.1534*S$
 $+ 0.273*Wt - 0.127*Age +$
 $4.56*Sex - 12.44,$ where 0 if
female and 1 if male

(Hannan et al. 1993): %FM =
 $+ 7.32 - 0.572*S^2/R +$
 $0.664*Wt$

(Stolarczyk et al. 1994): FFM
 $= 0.0012454*S^2 - 0.09404*R$
 $+ 0.1555*Wt + 0.1417*Xc -$
 $0.0833*Age + 20.05$

Hannan et al. (Hannan et al. 1993) equation showed no
difference in the %FM estimation (difference mean value: 0.6
%).

Stolarczyk et al. (Stolarczyk et al. 1994) equation
underestimated FFM (difference mean value: -3.6 kg)

| | | | | | | | |
|--------------------------|-----------------|---|---|----------|---|----------------------|--|
| (Williams and Bale 1998) | Cross-sectional | 232 athletes (men: n = 117, age 21.2 ± 1.2 y and women: n = 115, age 21.1 ± 1.3 y) involved in different sports | 101, RJL Systems, Detroit, MI / BIA using a foot to hand technology at single frequency | 50 / 800 | Equations owned by manufacturer | Hydrostatic weighing | BIA overestimated %FM in men (difference mean value: 0.9 %; LoA: -6.2 to 3.8) and women (difference mean value: 1.2 %; LoA: -3.2 to 4.8) |
| (Fornetti et al. 1999) | Cross-sectional | 132 female athletes (age 20.4 ± 1.5 y) involved in different sports | 101, RJL Systems, Detroit, MI / BIA using a foot to hand technology at single frequency | 50 / 800 | FFM = (0.282*S) + (0.415*Wt) – (0.037*R) + (0.096*Xc) – 9.734 | DXA | BIA's equation showed no difference in the FFM estimation (difference mean value: -0.1 kg) |
| (De Lorenzo et al. 2000) | Cross-sectional | 43 male athletes (19 water polo, 9 judo, 15 karate) aged 18 -34 y | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | (Oppliger et al. 1991): %FM = [(Wt – FFM)/Wt] * 100, with FFM = 1.949 + (0.701*Wt) + 0.186* (S ² /R) | DXA | BIA underestimated %FM (difference mean value: -2.5 %; LoA: -8.0 to 3.0) and overestimated FFM (difference mean value: 2.4 kg; LoA: -4.5 to 9.0) |
| (Houtkoo pr et al. 2001) | Cross-sectional | 19 female heptathletes (age 25.5 ± 3.5 y) | Valhalla 1990B, Valhalla, San Diego, CA/ BIA using a foot to hand technology at single frequency | 50 / 800 | (Lohman 1992): %FM = [(Wt – FFM)/Wt] * 100, with FFM = [0.73*(S ² /R)] + (0.16*Wt) + 2.0 (Lohman 1992): %FM = [(Wt – FFM)/Wt] * 100, with FFM = [0.666 (S ² /R)] + (0.217*Xc) + (0.164*Wt) – 8.78 Equation owned by Valhalla Impedance Analyzer Corp. | DXA | Lohman's (Lohman 1992) equation overestimated %FM (difference mean value: 2.1 %) Lohman's (Lohman 1992) equation overestimated %FM (difference mean value: 1.8 %) Equation owned by Valhalla Impedance Analyzer Corp. overestimated %FM (difference mean value: 5.5 %) Lukaski and Bolonchuk (Lukaski and Bolonchuk 1987) equation overestimated %FM (difference mean value: 4.4 %) |

(Lukaski and Bolonchuk 1987): %FM = [(Wt – FFM)/Wt] * 100, with FFM = 0.734*S²/R + 0.116*Wt + 0.096*Xc + 0.876*Sex – 4.03, where 0 if female and 1 if male

| | | | | | | | |
|------------------------|-----------------|--|--|-----------|---|--|---|
| (Civar et al. 2003) | Cross-sectional | 99 male (age 21.87 ± 2.04 y) athletes involved in different sports | Tanita 310, Tanita Inc., Tokyo, Japan / BIA using a leg to leg technology at multifrequency | N/A / N/A | Equations owned by manufactures | Hydrostatic weighing | BIA underestimated %FM (difference mean value: 3.2 %) |
| (Andreoli et al. 2004) | Cross-sectional | 10 male (age 21.0 ± 4.3 y) water polo athletes. | Xitron 4000b, Xitron technologies, San Diego, CA / BIS using a foot to hand technology at multifrequency | 50 / 500 | (Oppliger et al. 1991): %FM = [(Wt – FFM)/Wt] * 100, with FFM = 1.949 + (0.701*Wt) + 0.186* (S ² /R) | 4C according to the Withers et al. (1998) equation | BIS overestimated %FM (difference mean value: 12.1 %) |
| (Dixon et al. 2005) | Cross-sectional | 25 male wrestlers (age 19.2 ± 1.2 y) | TBF-300A, Tanita Corp., Arlington Heights, IL / BIA using a leg to leg technology at multifrequency | N/A / N/A | “Athletic” equation owned by manufactures | Hydrostatic weighing | BIA underestimated FM (difference mean value: - 2.2 kg; LoA: -5.0 to 9.4) |
| (Civar et al. 2006) | Cross-sectional | 60 female (age 20.70 ± 1.43 y) athletes involved in different sports | Tanita 310, Tanita Inc., Tokyo, Japan / BIA using a leg to leg technology at multifrequency | N/A / N/A | Equations owned by manufactures | Hydrostatic weighing | BIA showed no difference in the FM estimation (difference mean value: 0.2 kg) |

| | | | | | | | |
|--------------------------|-----------------|---|--|---|--|-----|---|
| (Svantesson et al. 2008) | Cross-sectional | 33 male athletes: 16 ice hockey players (age 15.6 ± 6.1 y) and 17 soccer players (age 24.1 ± 3.8 y) | Hydra 4200, Xitron technologies, San Diego, CA / BIS using a foot to hand technology at multifrequency | 5 - 1000 / 800 | Equations owned by manufactures | DXA | BIS underestimated FM (difference mean value: - 2.8 kg) and overestimated FFM (difference mean value: 2.0 kg) |
| (Company and Ball 2010) | Cross-sectional | 80 male athletes: 40 endurance athletes (age 30.4 ± 1.3 y) and 40 short distance runners (age 23.1 ± 0.7 y) | DF50, ImpediMed, San Diego, CA / BIA using a foot to hand technology at single frequency | 50 / 200 | (Lukaski et al. 1986): %FM = $[(Wt - FFM)/Wt] * 100$, with $FFM = 4.917 + 0.821 * S^2/R$ | DXA | BIA overestimated %FM (difference mean value: 6.4 %) |
| (Esco et al. 2011) | Cross-sectional | 40 female athletes (21.1 \pm 2.3) involved in different sports | HBF-300, Omron Helthcare, Kyot, Japan / BIA using a hand to hand technology at multifrequency | N/A / N/A | Equations owned by manufacturer | DXA | BIA underestimated %FM (difference mean value: -5.1 %, LoA: -2.2 to 12.3) and overestimated FFM (difference mean value: 3.4 kg, LoA: -2.4 to 8.4) |
| (Loenneke et al. 2012) | Cross-sectional | 33 male (age 20.0 ± 1.0 y) baseball players and 16 female (age 20.0 ± 1.0 y) gymnasts | HBF-500, Omron Helthcare, Kyoto, Japan / BIA using a direct segmental technology at multifrequency | N/A / N/A | FFM index = FFM/S^2 , with FFM estimated using an equation owned by manufactures | DXA | BIA underestimated FFM index in men (difference mean value: 0.5 kg/m^2) and women (difference mean value: 1.2 kg/m^2) |
| (Loenneke et al. 2013) | Cross-sectional | 35 male (age 20.1 ± 1.0 y) baseball players | i) TBF-350, Tanita Corp., Arlington Heights, IL / BIA using a leg to leg technology at multifrequency | i) N/A / N/A ii) N/A / N/A iii) N/A / N/A | Two predictive equations provided by the manufacturer (“athletes” and “non-athletes”) Two predictive equations provided by the manufacturer | DXA | Leg to leg BIA with the “athletes” equation underestimated %FM (difference mean value: -5.5 %), while no difference was found using the “non-athletes” equation (difference mean value: 0.2 %) Hand to hand BIA with the “athletes” equation underestimated %FM (difference mean value: -5.7 %), while no difference was |

| | | | | | | | |
|-------------------------|-----------------|--|--|----------------|---|-----|---|
| | | | ii) HBF-306, Omron Helthcare, Kyoto, Japan / BIA using a hand to hand technology at multifrequency | | (“athletes” and “non-athletes”) Equation owned by the manufacturer | | found using the “non-athletes” equation (difference mean value: 0.6 %) Direct segmental BIA overestimated %FM (difference mean value: 2.0 %) |
| | | | ii) HBF-500, Omron Helthcare, Kyoto, Japan / BIA using a direct segmental technology at multifrequency | | | | |
| (Birzniece et al. 2015) | Longitudinal | 71 athletes (men: n = 43, age 27.1 ± 0.8 y and women: n = 28, age 29.4 ± 1.2 y) involved in different sports | SFB7, ImpediMed, Brisbane, Australia / BIS using a foot to hand technology at multifrequency | 4 – 1000 / 200 | FFM = total body water/0.732, with TBW estimated using an equation owned by the manufacturer FM = Wt – FFM | DXA | BIS underestimated FM (difference mean value: -3.9 kg, LoA: -2.5 to 15.0) and overestimated FFM (difference mean value: 7.2 kg, LoA: -17.0 to 0.1) at baseline considering the athletes as an entire group BIS underestimated change in FM (difference mean value: -1.2 kg, LoA: -4.5 to 11.0) and overestimated change in FFM (difference mean value: 1.0 kg, LoA: -11.0 to 4.0) considering the athletes as an entire group |
| (Esco et al. 2015) | Cross-sectional | 45 female athletes (age 21.2 ± 2.0 y) involved in different sports. | InBody 770, Biospace, Co, Seoul, Korea / BIA using a direct segmental technology at multifrequency | 5 – 500 / N/A | Equations owned by manufacturers | DXA | BIA underestimated %FM (difference mean value: -3.3 %, LoA: 2.3 to -8.9) and overestimated FFM (difference mean value: 2.2 kg, LoA: -1.6 to -0.1) BIA showed no difference in the arms (difference mean value: 0.1 kg, LoA: 0.7 to -0.8), legs (difference mean value: 0.3 kg, LoA: 2.2 to -3.0), trunk (difference mean value: 0.1 kg, LoA: 3.3 to -3.0), and total LST (difference mean value: 0.2 kg, LoA: 4.0 to -4.4) estimation. |

| | | | | | | | |
|------------------------|-----------------|---|--|----------------------------------|----------------------------------|-----|--|
| (Krzykała et al. 2016) | Cross-sectional | 31 female field hockey players (age 19.5 ± 3.6 y) | i) 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency ii) BC418, Tanita Corp., Arlington Heights, IL / BIA using a direct segmental technology at multifrequency | i) 50 / 400 ii) N/A / N/A | Equations owned by manufacturers | DXA | Foot to hand BIA showed no difference in the %FM estimation (difference mean value: 0.1 %, LoA: 8.0 to -8.5) Direct segmental BIA underestimated %FM (difference mean value: -4.9 %, LoA: 2.0 to -11.0). |
| (Raymond et al. 2018) | Cross-sectional | 44 male (age 19.0 ± 1.0 y) American football athletes | InBody 770, Biospace, Co, Seoul, Korea / BIA using a direct segmental technology at multifrequency | 1 – 1000 / N/A | Equations owned by manufactures | DXA | BIA underestimated arms FM (difference mean value: -0.4 kg, LoA: -1.1 to 1.8), arms %FM (difference mean value: -1.9 %, LoA: -7.9 to 11.9), and arms FFM (difference mean value: -1.4 kg, LoA: -0.4 to 3.2) BIA underestimated legs FM (difference mean value: -2.8 kg, LoA: 3.3 to 11.3), legs %FM (difference mean value: -3.9 %, LoA: -1.0 to 6.7), and legs FFM (difference mean value: -5.4 kg, LoA: 0.7 to 9.9) BIA showed no difference in FM (difference mean value: 0.2 kg, LoA: -6.2 to 5.7) and FFM (difference mean value: -0.4 kg, LoA: -4.3 to 5.1) and in %FM estimation (difference mean value: 0.9 %, LoA: -10.0 to 8.7) of the trunk BIA underestimated FM (difference mean value: -3.0 kg, LoA: -4.4 to 10.4) and %FM (difference mean value: -2.5 %, LoA: - |

| | | | | | | | |
|----------------------------|-----------------|--|--|--|--|--|--|
| (Brewer et al. 2019) | Cross-sectional | 160 athletes involved in different sports: 44 men and 116 women (aged from 18 to 23 y) | InBody 770, Biospace, Co, Seoul. Korea / BIA using a direct segmental technology at multifrequency | N/A / N/A | Equations owned by manufacturer | DXA | 7.9 to 12.9), and overestimated FFM (difference mean value: 2.5 kg, LoA: -11.3 to 6.4) BIA underestimated legs (men: difference mean value: -6.6 kg; LoA: -15.3 to 3.2; women: difference mean value: -2.7 kg; LoA: -5.9 to 0.4) FM, while showed no difference in arms FM (men: difference mean value: 0.6 kg; LoA: -2.4 to 3.5; women: difference mean value: -0.1 kg; LoA: -0.9 to 0.8) BIA underestimated arms (men: difference mean value: -1.3 kg; LoA: -3.1 to 0.5; women: difference mean value: -0.4 kg; LoA: -1.4 to 0.5) and legs (men: difference mean value: -6.6 kg; LoA: -15.3 to 3.2; women: difference mean value: -2.7 kg; LoA: -5.9 to 0.4) FFM |
| (Domingos et al. 2019) | Cross-sectional | 29 male (age 23.1 ± 3.4 y) judo athletes | TBF-310 Tanita, Tanita Corp., Tokyo, Japan / BIA using a leg to leg technology at multifrequency | N/A / N/A | Equation owned by manufactures | 4C according to the Withers et al. (1998) equation | BIA overestimated FM (difference mean value: 1.2 kg, LoA: -6.7 to 7.0) |
| (Arias Téllez et al. 2019) | Cross-sectional | 30 male climbers (age 26.1 ± 4.9 y) | QuadScan 4000, Bodystat, Douglas, UK / BIA using a foot to hand technology at multifrequency | N/A / N/A | Two predictive equations owned by the manufacturer (“athletes” and “non-athletes”) | DXA | The “athletes” equation underestimated %FM (difference mean value: -6. %2, LoA: -11.8 to -0.7). The “non-athletes” equation underestimated %FM (difference mean value: -9.2 %, LoA: -13.6 to -4.74) |
| (Graybeal et al. 2020) | Cross-sectional | 27 bodybuilders (men: n = 17, age 26.0 ± 6.5 y and women: n = 10, age 25.8 ± 5.4 y). | i) SFB7, ImpediMed, Carlsbad, CA, USA / BIS using a foot to hand technology at | i) 3 - 1000 / 200 ii) N/A / N/A iii) N/A / N/A | Equations owned by manufacturers | 4C according to the Wang et al. (2002) equation | BIS showed no difference in the FM (men: difference mean value: -0.9 kg; women: difference mean value: -0.8) and FFM estimation (men: difference mean value: -0.4 kg; women: difference mean value: 1.3) |

multifrequency iv) N/A / N/A

ii) mBCA 514/515,
Seca, Hamburg,
Germany / BIA
using a direct
segmental
technology at
multifrequency

iii) TBF-300A
Tanita, Tanita
Corp., Tokyo, Japan
/ BIA using a leg to
leg technology at
multifrequency

iv) HBF-306,
Omron, Kyota,
Japan / BIA using a
hand to hand
technology at
multifrequency

Direct segmental BIA overestimated FM (difference mean value: 4.3 kg) in men and showed no difference for women (difference mean value: 0.6 kg). Direct segmental BIA underestimated FFM (difference mean value: -4.3 kg) in men and showed no difference for women (difference mean value: -0.6 kg).

Leg to leg BIA overestimated FM (difference mean value: 5.1 kg) in men and showed no difference for women (difference mean value: 2.3 kg). Leg to leg BIA underestimated FFM (difference mean value: -4.3 kg) in men and showed no difference for women (difference mean value: -1.8 kg).

Hand to hand BIA overestimated FM (difference mean value: 3.3 kg) in men and showed no difference for women (difference mean value: 0.2 kg). Hand to hand BIA underestimated FFM (difference mean value: -3.3 kg) in men and showed no difference for women (difference mean value: 0.7 kg).

| | | | | | | | |
|-------------------------------------|---------------------|---|--|-----------|------------------------------------|----------------|---|
| (Hartman n Nunes et al. 2020) | Cross- sectional | 19 male rugby players (age 25.2 ± 3.6 y) | InBody 720, Biospace, Co, Seoul. Korea / BIA using a direct segmental technology at multifrequency | N/A / N/A | Equations owned by manufacturer | ADP DXA | BIA overestimated FM (difference mean value: -0.8 kg; LoA: -13.5 to 11.5) and underestimated FFM (difference mean value: -0.9 kg; LoA: -13.7 to 11.7) compared to ADP BIA overestimated FM (difference mean value: 4.3 kg; LoA: -2.8 to 11.7) and underestimated FFM (difference mean value: -8.1 kg; LoA: -16.4 to 0.3) compared to DXA |
|-------------------------------------|---------------------|---|--|-----------|------------------------------------|----------------|---|

| | | | | | | | |
|------------------------|-----------------|--|--|--|---|--------------------------------|--|
| (Sardinha et al. 2020) | Cross-sectional | 88 athletes (men: n = 56, age 22.3 ± 4.3 y and women: n = 32, age 22.9 ± 5.2 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | Arms LST = 0.940*Sex + 0.042*Wt + 0.080*S ² /R + 0.024*Xc - 3.927, where Sex is 1 if female or 0 if male Legs LST = 1.983*Sex + 0.154*Wt + 0.127*S ² /R - 1.147, where Sex is 1 if female or 0 if male | DXA | BIA's equations showed no difference in the arms (difference mean value: 0.1 kg, LoA: -1.1 to 1.3) and legs (difference mean value: 0.1 kg, LoA: -3.8 to 3.9) LST estimation |
| (Lee et al. 2021) | Cross-sectional | 95 athletes (men: n = 50, age 23.0 ± 1.6 y and women: n = 45, age 24.0 ± 3.6 y) involved in different sports | i) IOI353, Jawon Medical, Gyeongsan, Korea / BIA using a direct segmental technology at multifrequency ii) InBody 230, Biospace, Co, Seoul. Korea / BIA using a direct segmental technology at multifrequency iii) InBody 770, Biospace, Co, Seoul. Korea / BIA using a direct segmental | i) 5 - 250 / 250 ii) 20 -100 / 330 iii) 1 -1000 / 80 | Equations owned by manufacturer | DXA Computed tomography | Two direct segmental devices overestimated %FM (IOI353: difference mean value: 0.6 %, LoA: -2.9 to 4.3; InBody 230: difference mean value: -0.7 %, LoA: -3.2 to 3.8) compared to DXA in men All the direct segmental devices overestimated %FM (IOI353: difference mean value: 2.2 %, LoA: -7.5 to 3.2; InBody 230: difference mean value: -1.6 %, LoA: -5.6.0 to 2.6; InBody 770: difference mean value: 2.4 %, LoA: -6.4 to -2.0) compared to DXA in women All the direct segmental devices overestimated absolute visceral body fat compared to computed tomography in men (IOI353: difference mean value: 21.0 kg, LoA: -20.6 to 62.6; InBody 230: difference mean value: 10.1 kg, LoA: -29.6 to 49.7; InBody 770: difference mean value: 9.2 kg, LoA: -33.4 to 55.0) and in women (IOI353: difference mean value: 9.9 kg, LoA: -20.6 to 62.6; InBody 230: difference mean value: 23.4 kg, LoA: -29.6 to 49.7; InBody 770: difference mean value: 31.2 kg, LoA: -33.4 to 55.0) |

| | | | | | | | |
|--------------------------|-----------------|--|---|-----------|---|---|---|
| | | | technology at multifrequency | | | | |
| (Matias et al. 2021) | Cross-sectional | 47 athletes (men: n = 33, age 21.9 ± 4.7 and women: n = 14, age 24.9 ± 6.0) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | FFM = -2.261 + 0.327*S ² /R + 0.525*Wt + 5.462*Sex, where Sex is 1 if female or 0 if male. | 4C according to the Wang et al. (2002) equation | BIA's equations showed no difference in the FFM estimation (difference mean value: -1.5 kg, LoA: -7.8 to 4.7) |
| (Syed-Abdul et al. 2021) | Cross-sectional | 104 male American football players (age 19.6 ± 1.5 y) | HBF-306, Omron, Kyota, Japan / BIA using a hand to hand technology at multifrequency | N/A / N/A | Two predictive equations owned by the manufacturer ("athletes" and "non-athletes") | DXA | The "athletes" equation underestimated %FM (difference mean value: -4.7 %, LoA: -14.1 to 4.7) The "non-athletes" equation showed no difference in the %FM estimation (difference mean value: -0.4 %, LoA: -8.5 to 7.7) |

Note: Data are shown as mean ± standard deviation. BIA: bioimpedance analysis; BIS: bioimpedance spectroscopy; N/A: not available; LoA: limits of agreements; DXA: Dual-energy X-ray Absorptiometry; ADP: Air displacement plethysmography; R: resistance; Xc: reactance; LST: lean soft tissue; FFM: fat-free mass; FM: fat mass; TBW: total body water; Wt: weight in kilograms; S: stature in meters; 4C: four-component model.

Table 2. Articles comparing bioimpedance outcomes with total body, extra and intra cellular water derived using a reference method.

| Authors | Study design | Participants | Bioimpedance device / method | Sampling frequency (kHz) / Current (μ A) | Analytical procedure | Reference method | Main results |
|-------------------------|--------------|--|--|---|---|--------------------|--|
| (Birzniece et al. 2015) | Longitudinal | 71 athletes (men: n = 34, age 27.1 ± 0.8 y and women: n = 37, age 29.4 ± 1.2 y) involved in different sports | SFB7, ImpediMed, Brisbane, Australia / BIS using a foot to hand technology at multifrequency | 4 – 1000 / N/A | Equation owned by the manufacturer | Bromide dilution | BIS underestimated ECW (difference mean value: -3.5 L, LoA: -3.5 to 3.0) considering the athletes as an entire group BIS showed no difference in the estimation of ECW change considering the athletes as an entire group |
| (Deminice et al. 2016) | Longitudinal | 13 male soccer players (age 18.2 ± 0.8 y) divided into creatine supplementation and placebo groups | 310E, Biodynamics, Seattle, USA / BIA using a foot to hand technology at single frequency | 50 / N/A | (Lukaski and Bolonchuk 1988): $TBW = 0.372*S^2/R + 3.05*Sex + 0.142*Wt - 0.069*Age$, where Sex is 1 if men and 0 if female* (Kushner and Schoeller 1986): $TBW = 8.399 + 0.396*S^2/R + 0.143*Wt$ (Kushner et al. 1992): $TBW = 0.59*S/R + 0.065*Wt + 0.04$ (Deurenberg et al. 1990): $TBW = 6.53 + 0.36740*S^2/impedance + 0.17531*Wt - 0.11 + Age + 2.83*Sex$, where Sex is 1 if men and 0 if female* | Deuterium dilution | Lukaski and Bolonchuk (Lukaski and Bolonchuk 1988) equation underestimated change in TBW in control (difference mean value: -1.2 L) and creatine supplementation groups (difference mean value: -1.1 L) Kushner and Schoeller (Kushner and Schoeller 1986) equation underestimated change in TBW in control (difference mean value: -1.0 L) and creatine supplementation groups (difference mean value: -1.1 L) Kushner et al. (Kushner et al. 1992) equation underestimated change in TBW in control (difference mean value: -1.2 L) and creatine supplementation groups (difference mean value: -0.9 L) Deurenberg et al. (Deurenberg et al. 1990) equation underestimated change in TBW in control (difference mean value: -1.3 L) and creatine supplementation groups (difference mean value: -1.1 L) |

(Morgenstern et al. 2002):
 $TBW = 0.0758 * 0.84^{[if\ female]}$
 $*(S * Wt)^{0.69}$

Morgenstern et al. (Morgenstern et al. 2002) equation underestimated change in TBW in control (difference mean value: -0.2 L) and creatine supplementation groups (difference mean value: -1.9 L)

(Sun et al. 2003): $TBW = 1.20 + 0.45 * S^2 / R + 0.18 * Wt$

Sun et al. (Sun et al. 2003) equation underestimated change in TBW in control (difference mean value: -1.0 L) and creatine supplementation groups (difference mean value: -1.1 L)

| | | | | | | | |
|-----------------------|-----------------|--|--|-----------------------------|---|--------------------------------|---|
| (Matias et al. 2016a) | Cross-sectional | 184 athletes (men: n = 127, age 16–38 y and women: n = 57, age 16–35 y) involved in different sports | i) 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | i) 50 / 400 ii) 50 / 800 | Equation used by BIA: BodygramPRO3.0 (Akern Systems, Italy) predictive equations for the TBW, ECW, and ICW estimations | Deuterium and bromide dilution | BodygramPRO3.0 predictive equations showed no difference for the TBW (difference mean value: 0.1 L, LoA: -3.7 to 3.9), ECW (difference mean value: -0.3 L, LoA: -3.0 to 2.4), and ICW (difference mean value: 0.6 L, LoA: -3.4 to 4.7) estimations in women, while underestimated TBW (difference mean value: -1.2 L, LoA: -5.9 to 3.4), ECW (difference mean value: -0.4 L, LoA: -3.9 to 3.0), and ICW (difference mean value: -0.7 L, LoA: -6.2 to 4.7) in men Kushner and Schoeller (Kushner and Schoeller 1986) equation overestimated TBW in women (difference mean value: 1.7 L, LoA: -2.2 to 5.7), while showed no difference for the TBW estimation in men (difference mean value: 0.4 L, LoA: -5.2 to 5.9) Van Loan and Mayclin (Van Loan and Mayclin 1987) equation overestimated TBW in women (difference mean value: 2.6 L, LoA: 2.3 to 7.6), while underestimated TBW in men (difference mean value: -5.3 L, LoA: -11.5 to 0.8) Lukaski and Bolonchuk (Lukaski and Bolonchuk 1988) equation underestimated TBW in women (difference mean value: -3.4 L, LoA: -7.3 to -0.5) and men (difference mean |
| | | | ii) Hydra 4200, Xitron Technologies, San Diego, CA / BIS using a foot to hand technology at multifrequency | | (Kushner and Schoeller 1986): $TBW = 8.399 + 0.396 * S^2 / R + 0.143 * Wt$ | | |
| | | | | | (Van Loan and Mayclin 1987): $TBW = 9.9868 + 0.000724 * S^2 + 0.2822 * Wt - 0.0153 * R - 2.3313 * Sex - 0.1319 * Age$ | | |
| | | | | | (Lukaski and Bolonchuk 1988): $TBW = 0.377 * S^2 / R + 0.14 * Wt - 0.08 * age + 2.9 * Sex + 4.65$, where Sex is 0 if female and 1 if male; ECW | | |

$$= 0.189*(S^2/R) + 0.052*Wt - 0.0002*(S^2/Xc) + 1.03$$

(Kushner et al. 1992): TBW = $0.59* S/R + 0.065*Wt + 0.04$

(Schoeller and Luke 2000):
TBW = $0.499*S^2/R + 0.080*Wt + 2.9$

(Sun et al. 2003): TBW = $1.20 + 0.45*S^2/R + 0.18*Wt$ for men and TBW = $3.75 + 0.45*S^2/R + 0.11*Wt$ for women

(Sergi et al. 1994) :ECW = $-5.22 + 0.2*S^2/R + 0.005/Xc + 0.08*Wt + 1.9 + 1.86*Sex$, where Sex is 0 if female and 1 if male

Equations used by BIS:

Equations owned by manufacturer for the TBW, ECW, and ICW estimations

value: -5.1 L, LoA: -9.9 to -0.1). Lukaski and Bolonchuk (1988) equation underestimated ECW in women (difference mean value: -0.7 L, LoA: -3.0 to -1.6) and men (difference mean value: -0.4 L, LoA: -3.3 to 2.4)

Kushner et al. (Kushner et al. 1992) equation showed no difference in the TBW estimation in women (difference mean value: -0.1 L, LoA: -4.2 to 3.9), while underestimated TBW in men (difference mean value: -1.2 L, LoA: -7.0 to 4.6).

Schoeller and Luke (Schoeller and Luke 2000) equation underestimated TBW in women (difference mean value: -1.0 L, LoA: -4.8 to 2.0) and men (difference mean value: -3.7 L, LoA: -9.0 to 1.5).

Sun et al. (Sun et al. 2003) equation underestimated TBW in women (difference mean value: -0.8 L, LoA: -4.6 to 2.9) and men (difference mean value: -1.4 L, LoA: -6.2 to 3.5)

Sergi et al. (Sergi et al. 1994) equation underestimated ECW in women (difference mean value: -2.7 L, LoA: -5.0 to 0.1), while showed no difference in men (difference mean value: 0.0 L, LoA: -4.0 to 3.9)

BIS underestimated TBW in women (difference mean value: -0.3 L, LoA: -2.0 to 1.4) while showed no difference in men. BIS underestimated ECW in women (difference mean value: -0.6 L, LoA: -2.7 to 1.5) while showed no difference in men. BIS showed no difference in the ICW estimation in men and women.

| | | | | | | | |
|-----------------------|-----------------|--|---|----------|---|--------------------------------|--|
| (Matias et al. 2016b) | Cross-sectional | 69 athletes (men: n = 46, age 22.5 ± 5.3 y and women: n = 23, age 20.8 ± 5.4 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | (Matias et al. 2016b): $TBW = 0.286 + 0.195 * S^2/R + 0.385 * Wt + 5.086 * Sex$, where Sex is 0 if female and 1 if male; $ECW = 1.579 + 0.055 * S^2/R + 0.127 * Wt + 0.006 * S^2/Xc + 0.932 * Sex$, where Sex is 0 if female and 1 if male; $ICW = TBW - ECW$ | Deuterium and bromide dilution | Matias et al. (Matias et al. 2016b) equation showed no difference in the TBW (difference mean value: -0.0 L, LoA: -5.6 to 5.6), ECW (difference mean value: 0.2 L, LoA: -3.6 to 4.0), and ICW (difference mean value: -0.2 L, LoA: -6.5 to 6.1) estimations Kushner and Schoeller (Kushner and Schoeller 1986) equation showed no difference in the TBW estimation (difference mean value: 0.3 L, LoA: -5.8 to 6.3) Van Loan & Mayclin (Van Loan and Mayclin 1987) equation underestimated TBW (difference mean value: -3.1 l, LoA: -13.1 to 7.0) Lukaski and Bolonchuk (Lukaski and Bolonchuk 1988) equation underestimated TBW (difference mean value: -3.6 L, LoA: -8.5 to 13.0) and ECW (difference mean value: -0.8 L, LoA: -4.7 to 3.0) Kushner et al. (Kushner et al. 1992) equation underestimated TBW (difference mean value: -1.5 L, LoA: -7.7 to 4.7) Schoeller and Luke (Schoeller and Luke 2000) equation underestimated TBW (difference mean value: -3.5 L, LoA: -9.9 to 3.0) Sun et al. (Sun et al. 2003) equation underestimated TBW (difference mean value: -1.6 L, LoA: -6.9 to 3.8) |
| | | | | | (Kushner and Schoeller 1986): $TBW = 8.399 + 0.396 * S^2/R + 0.143 * Wt$ | | |
| | | | | | (Van Loan and Mayclin 1987): $TBW = 9.9868 + 0.000724 * S^2 + 0.2822 * Wt - 0.0153 * R - 2.3313 * Sex - 0.1319 * Age$ | | |
| | | | | | (Lukaski and Bolonchuk 1988): $TBW = 0.377 * S^2/R + 0.14 * Wt - 0.08 * age + 2.9 * Sex + 4.65$, where Sex is 0 if female and 1 if male; $ECW = 0.189 * (S^2/R) + 0.052 * Wt - 0.0002 * (S^2/Xc) + 1.03$ | | |

(Kushner et al. 1992): $TBW = 0.59 * S/R + 0.065 * Wt + 0.04$

Sergi et al. (Sergi et al. 1994) equation underestimated TBW (difference mean value: -0.9 L, LoA: -4.6 to 3.1)

(Schoeller and Luke 2000) $TBW = 0.499 * S^2/R + 0.080 * Wt + 2.9$

(Sun et al. 2003): $TBW = 1.20 + 0.45 * S^2/R + 0.18 * Wt$ for men and $TBW = 3.75 + 0.45 * S^2/R + 0.11 * Wt$ for women

(Sergi et al. 1994): $ECW = -5.22 + 0.2 * S^2/R + 0.005/Xc + 0.08 * Wt + 1.9 + 1.86 * Sex$, where Sex is 0 if female and 1 if male

| | | | | | | | |
|----------------------|-----------------|---|--|----------------|---|--------------------|---|
| (Shiose et al. 2020) | Cross-sectional | 18 male wrestler (age 21.0 ± 1.0 y) | SFB7, ImpediMed, Pinkenba, Australia / BIS using a foot to hand technology at multifrequency | 3 – 1000 / 200 | (De Lorenzo et al. 1997): $TBW = ECW + ICW$, with $ECW = 1/1000 * [(4.3^{2*}40.5^2)/(1.05 * 10^{-3})]^{1/3} * [(\sqrt{Wt} * S^2)^{extracellular}]^{2/3}$ and $ICW = 1 + (ICF^{bis}/ECW)^{5/2} = [(extracellularR + intracellularR)^{extracellularR}] * [1 + (273.9/40.5) * (ICF^{bis}/ECW)]$ | Deuterium dilution | De Lorenzo et al. (De Lorenzo et al. 1997) equation showed no difference in the TBW estimation (difference mean value: 0.3 L, LoA: -1.1 to 1.7) Moissl et al. (Moissl et al. 2006) equation showed no difference for the TBW estimation (difference mean value: 0.2 L, LoA: -1.0 to 1.4) |
| | | | | | (Moissl et al. 2006): $TBW = ECW + ICW$, with $ECW =$ | | |

| | | | | | | | |
|-------------------------|-----------------|---|---|----------|--|--------------------------------|---|
| | | | | | $[(0.188/\text{BMI}) + 0.2883] * [(S^2 * W_t^{1/2}) / \text{extracellular R}]^{2/3}$ $\text{and ICW} = [(0.58758/\text{BMI}) + 0.4194] * [(S^2 * W_t^{1/2}) / \text{intracellular R}]^{2/3}$ | | |
| (Francisco et al. 2021) | Cross-sectional | 201 athletes (134 men, 67 women) with mean age 21.4 ± 5.1y divided into well-hydrated, euhydrated and dehydrated groups | Hydra 4200, Xitron Technologies, San Diego, CA / BIS using a foot to hand technology at multifrequency | 50 / 800 | Equations owned by manufacturer for the TBW, ECW, and ICW estimations | Deuterium and bromide dilution | <p>BIS showed no difference for the TBW estimation in well-hydrated (difference mean value: -0.2 L, LoA: -3.1 to 2.7), euhydrated (difference mean value: -0.3 L, LoA: -2.8 to 2.2), and dehydrated (difference mean value: 0.0 L, LoA: -1.9 to 2.0) athletes</p> <p>BIS showed no difference for the ECW estimation in well-hydrated (difference mean value: -0.1 L, LoA: -3.3 to 3.0), euhydrated (difference mean value: -0.1 L, LoA: -3.4 to 3.6), and dehydrated (difference mean value: -1.2 L, LoA: -6.2 to 3.7) athletes</p> <p>BIS showed no difference for the ICW estimation in well-hydrated (difference mean value: -0.1 L, LoA: -4.3 to 4.1), euhydrated (difference mean value: -0.1 L, LoA: -4.1 to 3.9), and dehydrated (difference mean value: 1.2 L, LoA: 3.7 to 6.3) athletes</p> |
| (Coratella et al. 2021) | Cross-sectional | 185 athletes (men: n = 132, age 21.7 ± 5.1 y; women: n = 53, age 20.3 ± 4.5 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | (Matias et al. 2016b): $\text{TBW} = 0.286 + 0.195 * S^2/R + 0.385 * W_t + 5.086 * \text{Sex}$, where Sex is 0 if female and 1 if male; $\text{ECW} = 1.579 + 0.055 * S^2/R + 0.127 * W_t + 0.006 * S^2/X_c + 0.932 * \text{Sex}$, | Deuterium and bromide dilution | Matias et al. (Matias et al. 2016b) equation showed no difference for the TBW estimation in women (difference mean value: -0.3 L, LoA: -2.9 to 2.3) and men (difference mean value: 0.1 L, LoA: -2.3 to 2.4). Matias et al. (Matias et al. 2016b) equation showed no difference for the ECW estimation in women (difference mean value: -0.3 L, LoA: -1.4 to 1.7) and men (difference mean value: -0.6 L, LoA: -2.7 to 1.5). |

where Sex is 0 if female and 1 if male; ICW = TBW – ECW

(Sun et al. 2003): TBW = $1.20 + 0.45 * S^2/R + 0.18 * Wt$ for men and TBW = $3.75 + 0.45 * S^2/R + 0.11 * Wt$ for women

(Schoeller and Luke 2000): TBW = $0.499 * S^2/R + 0.080 * Wt + 2.9$

(Kushner et al. 1992): TBW = $0.59 * S/R + 0.065 * Wt + 0.04$

(Kotler et al. 1996): TBW = Male: $0.58 * (S^{1.62}/impedance^{0.7}) * (1/1.35) + 0.32 * Wt - 3.66$ and Female: $0.76 * (S^{1.99}/impedance^{0.58}) * (1/18.91) + 0.14 * Wt - 0.86$

(Lukaski and Bolonchuk 1988): TBW = $0.377 * S^2/R + 0.14 * Wt - 0.08 * age + 2.9 * Sex + 4.65$, where Sex is 0 if female and 1 if male; ECW = $0.189 * (S^2/R) + 0.052 * Wt - 0.0002 * (S^2/Xc) + 1.03$

Sun et al. (Sun et al. 2003) equation underestimated TBW in women (difference mean value: -1.5 L, LoA: -5.1 to 2.1) and men (difference mean value: -1.8 L, LoA: -6.9 to 3.3).

Schoeller and Luke (Schoeller and Luke 2000) equation underestimated TBW in women (difference mean value: -1.7 L, LoA: -5.3 to 2.0) and men (difference mean value: -4.1 L, LoA: -9.5 to 1.3).

Kushner et al. (Kushner et al. 1992) equation underestimated TBW in women (difference mean value: -0.7 L, LoA: -4.3 to 2.3) and men (difference mean value: -1.4 L, LoA: -6.7 to 3.9).

Kotler et al. (Kotler et al. 1996) showed no difference for the TBW estimation in women (difference mean value: 0.5 L, LoA: -3.4 to 4.1) and men (difference mean value: -1.6 L, LoA: -7.1 to 3.4).

Lukaski and Bolonchuk (Lukaski and Bolonchuk 1988) equation underestimated TBW in women (difference mean value: -4.1 L, LoA: -8.1 to 0.2) and men (difference mean value: -5.4 L, LoA: -11.3 to 0.4). Lukaski and Bolonchuk (Lukaski and Bolonchuk 1988) equation underestimated ECW in women (difference mean value: -1.9 L, LoA: -3.6 to 0.1), while showed no difference in men (difference mean value: -0.1 L, LoA: -3.5 to 3.4).

Sergi et al. (Sergi et al. 1994) underestimated ECW in women (difference mean value: -2.3 L, LoA: -4.1 to 0.6) and men (difference mean value: -1.8 L, LoA: -5.4 to 1.2).

(Sergi et al. 1994) $ECW = -$
 $5.22 + 0.2 * S^2 / R + 0.005 / Xc +$
 $0.08 * Wt + 1.9 + 1.86 * Sex,$
where Sex is 0 if female and 1
if male

Note: Data are shown as mean \pm standard deviation. BIA: bioimpedance analysis; BIS: bioimpedance spectroscopy; N/A: not available; LoA: limits of agreements; R: resistance; Xc: reactance; TBW: total body water; ECW: extracellular water; ICW: intracellular water; Wt: weight in kilograms; S: stature in meters.

Table 3. Articles comparing bioimpedance vector outcomes with total body water and percentage of fat mass using a reference method.

| Authors | Study design | Participants | Bioimpedance device / method | Sampling frequency (kHz) / Current (μ A) | Analytical procedure | Reference method | Main results |
|----------------------|-----------------|---|--|---|---|---|--|
| (Campa et al. 2020) | Longitudinal | 58 athletes (men: n = 39, age 18.7 ± 4.0 y; women: n = 19, age 19.2 ± 6.0 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | R and Xc adjusted according to the Classic BIVA approach (adjusted for S) | Deuterium and bromide dilution | Reductions in vector length were associated with increases in TBW ($r = -0.718$, $p < 0.01$) considering the athletes as an entire group Phase angle was positively correlated with the change in ICW/ECW ratio ($r = 0.436$, $p < 0.01$) considering the athletes as an entire group |
| (Marini et al. 2020) | Cross-sectional | 202 athletes (men: n = 139 age 21.5 ± 5.0 y; women: n = 63 age 20.7 ± 5.1 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | R and Xc adjusted according to the Classic BIVA (adjusted for S) and the <i>Specific</i> BIVA (adjusted for body geometries) approaches | DXA Deuterium and Bromide dilution and 4C according to the Wang et al. (2002) equation | <i>Specific</i> vector length was positively correlated with %FM (men: $r = 0.569$, $p < 0.001$; women: $r = 0.773$, $p < 0.001$). Classic vector length was negatively correlated with TBW (men: $r = -0.880$, $p < 0.001$; women: $r = -0.829$, $p < 0.001$) Phase angle was positively correlated with the ICW/ECW ratio (men: $r = 0.493$, $p < 0.001$; women: $r = 0.408$, $p < 0.001$) |
| (Silva et al. 2020) | Longitudinal | 27 male judo athletes (age 23.2 ± 2.8 y) | Hydra 4200, Xitron Technologies, San Diego, CA, US / BIS using a foot to hand technology at multifrequency | 50 / N/A | R and Xc adjusted according to the Classic BIVA approach | Deuterium and Bromide dilution | Decreases in TBW were accompanied by vector elongations ($T^2=2.6$, $F=1.2$, $P=0.3$, Mahalanobis distance=0.39), and vice versa ($T^2=4.1$, $F=1.8$, $P=0.2$, Mahalanobis distance=0.64) Phase angle was positively correlated with the ICW/ECW ratio ($\beta = 0.050$, $p=0.004$) |

| | | | | | | | |
|----------------------|-----------------|---|---|----------|--|-----|--|
| (Campa et al. 2021a) | Longitudinal | 80 athletes of different sports (age 43.9 ± 9.2 y) including 27 women and 53 men | Xitron 4000b, Xitron technologies, San Diego, CA / BIS using a foot to hand technology at multifrequency | 50 / N/A | R and Xc adjusted according to the <i>Specific</i> BIVA approach | DXA | <i>Specific</i> vector length was associated with change in %FM ($r^2 = 0.246$; $p < 0.001$) considering the athletes as an entire group |
| (Stagi et al. 2021) | Cross-sectional | 50 athletes (25 men: age 24.37 ± 4.79 y; 25 women: age 24.32 ± 4.43 y) involved in different sports | 101 Anniversary, AKERN Systems; Florence, Italy / BIA using a foot to hand technology at single frequency | 50 / 400 | R and Xc adjusted according to <i>Specific</i> BIVA | DXA | Good agreement between DXA and BIVA ($F=14.89$, $p < 0.001$) in both sexes and all body segments. <i>Specific</i> vector length was positively correlated with %FM _{DXA} in the whole body and all body segments, and the phase angle was correlated with FFMI _{DXA} . |

Note: Data are shown as mean \pm standard deviation. BIA: bioimpedance analysis; BIS: bioimpedance spectroscopy; BIVA: bioelectrical impedance vector analysis; N/A: not available; R: resistance; Xc: reactance; TBW: total body water; ECW: extracellular water; ICW: intracellular water; FM: fat mass; Wt: weight in kilograms; S: stature in meters.



Click here to access/download
Supplementary Material
Supplementary Table 1.docx



Funding: This research project received no external funding.

Conflicts of interest/Competing interests: The authors declare no conflict of interest. Availability of data and material:

Not applicable

Ethics approval: Not applicable