

Alma Mater Studiorum Università di Bologna  
Archivio istituzionale della ricerca

Does Implant Design Influence Failure Rate of Lateral Unicompartmental Knee Arthroplasty? A Meta-Analysis

This is the final peer-reviewed author's accepted manuscript (postprint) of the following publication:

*Published Version:*

Fratini, S., Meena, A., Alesi, D., Cammisa, E., Zaffagnini, S., Marcheggiani Muccioli, G.M. (2022). Does Implant Design Influence Failure Rate of Lateral Unicompartmental Knee Arthroplasty? A Meta-Analysis. THE JOURNAL OF ARTHROPLASTY, 37(5), 985-992 [10.1016/j.arth.2022.01.068].

*Availability:*

This version is available at: <https://hdl.handle.net/11585/875783> since: 2024-02-16

*Published:*

DOI: <http://doi.org/10.1016/j.arth.2022.01.068>

*Terms of use:*

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>).  
When citing, please refer to the published version.

(Article begins on next page)

**Title: “Does implant design influence failure rate of lateral unicompartmental knee arthroplasty? A meta-analysis.”**

Authors: Fratini Stefano<sup>1</sup>, Meena Amit<sup>2</sup>, Alesi Domenico<sup>1</sup>, Cammisa Eugenio<sup>1</sup>, Zaffagnini Stefano<sup>1,3</sup>, Marcheggiani Muccioli Giulio Maria<sup>1,3</sup>

<sup>1</sup> 2nd Orthopaedic and Traumatologic Clinic, IRCCS Istituto Ortopedico Rizzoli, Via G.B. Pupilli 1, 40136, Bologna, Italy

<sup>2</sup> Central Institute of Orthopaedics, Vardhman Mahavir Medical College & Safdarjung Hospital, New Delhi, 110029, India

<sup>3</sup> University of Bologna, Via Zamboni, 33, 40126, Bologna, Italy

Corresponding author: Dr. Stefano Fratini, MD, [dr.stefano.fratini@gmail.com](mailto:dr.stefano.fratini@gmail.com)

Word count of the abstract: 229

Word count of the manuscript: 2698

# 1 **Does implant design influence failure rate of lateral unicompartmental knee arthroplasty? A** 2 **meta-analysis.**

## 3 **Abstract**

### 4 Background

5 Lateral unicompartmental knee arthroplasty (UKA) is a viable solution for isolated lateral  
6 compartment arthritis. Several prosthetic designs are available such as Fixed Bearing Metal-Backed  
7 (FB M-B), Fixed Bearing All Polyethylene (FB A-P), and Mobile Bearing Metal Backed (MB M-  
8 B) implants. The purpose of this meta-analysis is to compare failure rates of different prosthetic  
9 designs.

### 10 Methods

11 Preferred Reporting Items for Systematic Reviews and Meta-Analyses systematic review was  
12 conducted using 4 databases (MEDLINE, EMBASE, Cochrane, and PubMed) to identify all studies  
13 that investigate outcomes of lateral UKA. 21 studies met the inclusion criteria, and failure rates  
14 were compared by implant type and follow-up time separately in order to assess potential  
15 confounding factors. Two separate analyses have been performed among different implant designs  
16 (FB M-B *vs* FB A-P *vs* MB M-B) and different follow-ups (less than 5 years, between 5 and 10  
17 years, more than 10 years).

### 18 Results

19 The failure rate of FB M-B lateral UKA was significantly lower compared to other lateral  
20 unicompartmental knee arthroplasty designs present on the market (0,8% *vs* 8,6% and 7,1% for FB  
21 M-B, FB A-P and MB M-B, respectively). No significative difference among groups has been  
22 detected when comparing all implants with regard to follow-up time.

### 23 Conclusion

24 Considering actual evidence, for a surgeon approaching lateral UKA, the Fixed Bearing Metal  
25 Backed design is preferable, given the lower failure rates and subsequently a longer implant  
26 survivorship.

### 27 **Keywords**

28 Lateral, Unicompartmental, Knee, Arthroplasty, Survivorship, Meta-analysis

29

## 30 **Background**

31 Lateral unicompartmental knee arthroplasty (UKA) is an appealing alternative to total knee  
32 arthroplasty (TKA) for patients with isolated lateral compartment arthritis. Whilst degenerative

joint disease may affect any compartment of the knee, the isolated lateral compartment arthritis of the knee is less common and much more challenging to treat. It is estimated that only less than 1% of the total number of knee arthroplasty and only 5–10% of all unicompartmental knee replacements are performed for lateral compartment disease[1,2]. This number might be artificially low because the majority of surgeons prefer total rather than lateral unicondylar knee arthroplasty for the treatment of lateral compartment osteoarthritis[3]. Compared to TKA, UKA has several potential advantages, which include a less invasive procedure, improved postoperative range of motion, preservation of the cruciate ligaments, fat pad and bone stock, improved proprioception, increased patient satisfaction, earlier return to activities, shorter hospital stay, and fewer complications [4–9]. Moreover, it leaves the healthy contralateral tibiofemoral compartment intact.

Despite these benefits, lateral compartment knee arthroplasty is more difficult to perform than medial compartment UKA due to its anatomic and biomechanical characteristics. The lateral collateral ligament is looser than the medial ligament, and the lateral femoral condyle anteroposterior translation is deeper than the medial side.[10] Moreover, the lateral tibial plateau is rounder compared to the medial plateau, the lateral femoral condyle is smaller than the medial condyle, and the screw-home mechanism is far more significant on the lateral side [11,12]. All these anatomic and biomechanical characteristics lead to a technically challenging procedure, a more difficult surgical approach, a significantly longer learning curve, therefore the need to perform a large number of procedures to achieve the lowest reoperation rates, which have traditionally been higher in UKA compared with TKA surgery[13,14].

Because of the infrequency of this procedure, few studies describe the survivorship and the causes of failure in lateral UKA[15]. These studies mainly include case series that involve a small cohort of patients, further comprised by mixed data including medial UKA[16]. Nevertheless, the scarce evidence in literature has shown acceptable results for short and mid-term survivorship of lateral UKA with remaining concerns on the long-term survivorship together with difficulties about identifying the main reasons for failure. Hence it is fundamental to systematically examine failure rates, evaluate the etiology and the mechanism of lateral UKA failure to improve the understanding and the revision strategy of a failed lateral UKA.

Several prosthetic designs are commercially available, which differ concerning the bearing and the materials. They can be divided into three groups: Fixed Bearing All-Polyethylene (FB A-P), Fixed Bearing Metal-Backed (FB M-B), and Mobile Bearing Metal-Backed (MB M-B) implants.

64 To our knowledge, limited evidence is available in literature on survivorship in lateral UKA in  
65 relation to implant design. Therefore, we performed a systematic review and metanalysis, pooling  
66 failure rates of studies that reported lateral UKA survivorship. The aim of this study was to assess  
67 the different rates of lateral UKA failures with regard to implant design.

68

69 **Material and Methods**

70 Article Identification and Selection

71 This study was conducted in accordance with the 2009 Preferred Reporting Items for Systematic  
72 Reviews and Meta-Analyses (PRISMA) statement[17] (Fig.1). A systematic review of the literature  
73 regarding the existing evidence for survivorship and clinical outcomes of Lateral Unicompartmental  
74 Knee Arthroplasty (UKA) was performed using the Cochrane Central Register of Controlled Trials,  
75 PubMed, MEDLINE (2011-2021), and EMBASE. The queries were performed in April 2021. The  
76 literature search strategy included the following: (lateral[All Fields] AND ("arthroplasty,  
77 replacement, knee"[MeSH Terms] OR ("arthroplasty"[All Fields] AND "replacement"[All Fields]  
78 AND "knee"[All Fields]) OR "knee replacement arthroplasty"[All Fields] OR  
79 ("unicompartmental"[All Fields] AND "knee"[All Fields] AND "arthroplasty"[All Fields]) OR  
80 "unicompartmental knee arthroplasty"[All Fields])) AND ("2011/01/01"[PDat] :  
81 "2021/04/28"[PDat]).

82 Inclusion criteria were as follows: survivorship and/or failure rates stated for lateral  
83 unicompartmental knee arthroplasty, English language, minimum follow-up of 2 years for all  
84 patients in the cohort, minimum of 20 patients in each study cohort, study published within the last  
85 10 years, same implant used for all patients in each cohort, and human studies. We excluded  
86 cadaveric studies, animal studies, biomechanical reports, basic science articles, editorial articles,  
87 case reports, literature reviews, surgical technique descriptions, instructional courses, and tumors.

88 Two independent reviewers (S.F., A.M.) performed a review of the abstracts from all identified  
89 articles. Full-text articles were obtained for review, if necessary, to allow for a further assessment of  
90 inclusion and exclusion criteria. Additionally, all references from the included studies were  
91 reviewed and reconciled to verify that no relevant articles were missing from the systematic review.

92     Data Collection and Processing

93     The level of evidence of the studies was assigned according to the classification system specified by  
94     Wright et al.[18] Data were abstracted from the full text of all eligible articles using standardized  
95     data collection forms. Abstracted and recorded data included patient demographics, the follow-up  
96     period, the type of implant used, failure rates and/or survivorship rates. For continuous variables  
97     (e.g. age, follow-up), the means, SDs, interquartile ranges, and ranges were collected (if reported).  
98     Data were recorded into a custom spreadsheet using a modified information extraction table.

99     Literature Quality Evaluation

100    Two reviewers (S.F., A.M.) used a modified version of the Coleman methodology score (mCMS) to  
101    assess the methodological quality of each study. The 2-part mCMS grades cartilage-related studies  
102    based on 10 criteria. Part A includes the study size, mean follow-up, number of different surgical  
103    procedures, type of study, description of the surgical procedure, postoperative rehabilitation,  
104    participants' magnetic resonance imaging outcome, and participants' histological outcome. Part B  
105    includes the outcome criteria, procedure for assessing clinical outcomes, and description of the  
106    participant selection process. The maximum mCMS is 100, which indicates a study that largely  
107    avoids chance, biases, and confounding factors.

108    Statistical Analysis

109    The primary outcome of the meta-analysis was the difference in failure rate among the three groups  
110    of implants evaluated (FB A-P, FB M-B, and MB M-B). The statistical analysis and the forest plot  
111    was carried out according to Neyeloff et al. using Microsoft Excel (release 2103 16.0.13901.20400 /  
112    April 13, 2021).[19] The Mantel-Haenszel method was used to evaluate the expected value[20];  
113    Wilson's confidence intervals were preferred because of data sparsity, either in terms of event rates  
114    being low or study size being small; therefore the standard error estimates using inverse variance  
115    methods were considered inadequate.[21] With no heterogeneity, the estimation of the expected  
116    value and its 95% confidence interval (CI) was based on fixed-effect analysis of variance; the  
117    random effect model was used otherwise. Statistical heterogeneity was evaluated by the I-square  
118    statistic and Cochrane's Q.[22] The comparisons among groups were based on the z-score

transformation of the difference. The rationale is that, under a normal-distribution assumption, a 95% CI is 2\*1.96 standard error's (SE) wide; therefore it is possible to estimate the SE for each group from the CI around each expected value. Then, the SE for the difference between the two groups can be calculated as  $SE(B - A) = \sqrt{SE(B)^2 + SE(A)^2}$  and  $Z = \frac{(B-A)}{SE(B-A)}$ . The *p*-value of the difference can be carried out from the normal standard distribution and then corrected with the Bonferroni method for multiple comparisons. Two investigators independently assessed the risks of bias (low, high or unclear). Publication bias was also assessed using a funnel plot (Fig. 2). Subgroup analyses based on differences in the follow-up period were also performed to explore a potential source of heterogeneity. Three subgroups were accordingly created in each group: short-term (<5 years), midterm (5–10 years), and long-term (>10 years) follow-up.

129

## 130 **Results**

A total of 2215 studies were selected for the analysis. After a review of the titles, abstracts, full titles, and excluding the unrelated studies, 21 articles were selected as eligible for the final meta-analysis.[23–43] Four of the 21 studies were prospective trials, while the others were retrospective analyses. The mean follow-up period ranged from 3 to 14.2 years. Additional details about study characteristics and patient demographics can be found in Table 1.

Within the selected studies, the FB A-P implants were from two manufacturers: HLS Uni Evolution (Tournier) and AMC Uniglide (Corin); the FB M-B implants were from five manufacturers: Restoris MCK (Stryker), Sled UKA (Waldemar Link), Unicompartmental High Flex Knee (Zimmer), Miller-Galante Unicompartmental Knee (Zimmer), iUni G1 (Conformis), Respicci II UKA (Biomet), Vanguard M UKA (Biomet); the MB M-B implants were from two manufacturers: Oxford Doomed Lateral UKR (Zimmer Biomet), Preservation UKA (DePuy).

### 142 Failure rates analysis by implant design

A total of 3378 knees were examined, and 219 experienced failure and subsequent revision. The total failure rate was 5,0% (95% C.I. 3,1%-6,9%).  $I^2$  was 85% showing substantial heterogeneity;

145 therefore random effect was applied.[22] The FB A-P group showed a failure rate of 8,6% (95%  
146 C.I. 3,2%-14,1%) with an  $I^2=54\%$ ; therefore random effect was applied. The FB M-B group  
147 showed a failure rate of 0,8% (95% C.I. 0,0%-1,6%) with no heterogeneity; therefore fixed effect  
148 was applied. The MB M-B group showed a failure rate of 7,1% (95% C.I. 5,3%-8,9%) with an  
149  $I^2=52\%$ , therefore random effect was applied. Data are summarized in Table 2 and Figure 3.

150 Meta-analysis evaluation showed a statistically significant difference among groups FB M-B and  
151 FB A-P ( $p=0,024$ ) and among groups FB M-B and MB M-B ( $p<0,01$ ). No significative difference  
152 has been noted among FB A-P and MB M-B groups ( $p>0,99$ ). Bonferroni correction has been  
153 applied due to the comparison among the three groups. Data are summarized in Table 3.

#### 154 Failure rates analysis by mean follow-up

155 Twelve of the 21 studies had a mean follow-up between 3 and 5 years [24–26,29–  
156 32,35,36,38,41,43], six had a mean follow-up between 5 and 10 years[23,27,33,34,40,42] and three  
157 had a follow-up longer than 10 years [28,37,39]. The shortest follow-up group showed a failure rate  
158 of 3,9% (95% C.I. 1,6%-6,3%) with an  $I^2=87\%$ ; therefore random effect was applied. The 5-to-10  
159 years follow-up group showed a failure rate of 7,0% (95% C.I. 2,6%-11,4%) with an  $I^2=82\%$ ;  
160 therefore random effect was applied. Lastly, the longest follow-up group showed a failure rate of  
161 8,9% (95% C.I. 0%-18,7%) with an  $I^2=83\%$ , and again random effect was applied. Data are  
162 summarized in Table 4 and Figure 4.

163 Meta-analysis evaluation did now show any statistically significant difference among groups. Data  
164 are shown in Table 5.

#### 165 Reoperation and Failure

166 Reoperation and failure results were reported in all the studies included in the present analysis. Data  
167 is summarized in Appendix.

#### 168 **Discussion**



169 The most important finding of the present meta-analysis was that the failure rate of Metal-Backed  
170 Fixed Bearing lateral unicompartmental arthroplasty was significantly lower compared to other  
171 lateral unicompartmental knee arthroplasty designs present on the market (0,8% vs 8,6% and 7,1%  
172 for FB M-B, FB A-P and MB M-B respectively).

173 A recent systematic review and meta-analysis evaluating mobile vs fixed bearing UKAs found  
174 better survival rates for fixed bearing implants. The mobile bearing implants showed an  
175 approximately four times higher risk of revision than fixed bearing designs when used for lateral  
176 UKA.[44]

177 Burger et al. found similar observations in their work and stated that revision risk is lower with FB  
178 implants than MB ones in lateral UKAs. According to them the annual revision rate was 2.16 (95%  
179 CI 1,54-3,04), 1.81 (95% CI 0,98-3,34) and 0.94 (95% CI 0,66-1,33) for MB, domed MB and FB  
180 designs respectively.[45] A study from Dutch arthroplasty registry data also reported similar results  
181 where the use of Mobile Bearing lateral UKA was associated with increased revision rate.[46]

182 The lateral knee compartment shows a different behavior with regard to the medial side. During  
183 knee flexion, while the medial condyle remains relatively static on the anteroposterior (AP) plane  
184 with approximatively 1,5mm of translation, the lateral side presents an inherent instability and has a  
185 greater degree of freedom with an AP translation from 9 to 15mm.[47,48]

186 The less constrain on the lateral knee condyle increases the underlying risk of bearing dislocation  
187 for MB implants. A fixed bearing construct reduces the system complexity and the bearing  
188 instability, providing a simpler and stronger construct.

189 To decrease bearing dislocation incidences, domed mobile bearing tibial implants were introduced  
190 in order to require more distractive force before the polyethylene insert dislocates. Those implants  
191 have a convex tibial component augmented with biconcave bearings, compared to previous designs,  
192 which featured a flat tibial component. Although by using domed implants the dislocation rate was  
193 significantly decreased with respect to non-domed implants, it does not eliminate the chance of  
194 bearing dislocation. Therefore, various modifications have been introduced to address this issue,  
195 such as placing a screw in the intercondylar notch, even if further increasing the system  
196 complexity.[25,30,49]

197 When analyzing failures based on the type of implant used, it can be found that bearing dislocation  
198 is the main responsible for failure when mobile bearing implants are used, whereas osteoarthritis  
199 progression is responsible for most failures in fixed bearing implants. Polyethylene wear is not the  
200 main determinant for survivorship, presumably thanks to improvement in polyethylene  
201 manufacturing, processing, design, sterilization, and storage which significantly improved over the  
202 last few years. [16,50]

203 When evaluating Metal-Backed and All-Polyethylene designs, a very scarce bibliography can be  
204 found on lateral UKAs. Studies based on medial UKAs show superiority of Metal-Backed tibial  
205 implants over All-Polyethylene designs.[51,52] It has to be noted, however, that the biomechanics  
206 of the medial side, as previously discussed, is different with regard to the lateral side, and those  
207 benefits may or may be not noted in lateral UKAs.

208 Based on the few studies on Metal-Backed *vs* All-Polyethylene lateral UKAs, no significant  
209 differences has been noted [23,53,54], while an increased risk of bearing dislocation has been  
210 described. Another study by Gunther et al. using Mobile Bearing lateral UKAs showed a 10% rate  
211 of inlay dislocations.[55] This effect is most likely due to greater AP translation of the lateral side  
212 during knee flexion.[56] While this behavior can be cause for concerns, it has not been noted in  
213 more recent studies included in this analysis. [35]

214 The present study has some limitations. Studies available in literature are often of poor quality, with  
215 few patients and incomplete data. However, a complete literature search has been performed with  
216 the aim of providing a complete analysis.

217 Lateral UKAs are less implanted than medial UKAs and have strict indications, despite comparable  
218 survivorships being shown at short, medium and long follow-up. [57] The surgeon experience and  
219 the number of lateral UKA performed play an essential role in outcomes and failures. For this  
220 reason, the same studies have been evaluated with regard to follow-up time as well, mixing all the  
221 designs together for assessing a potential confounding factor. No significative differences have been  
222 noted when evaluating failure rates by follow-up, confirming that the simpler implant design  
223 provides the lowest failure rates.

224 As things stand today, for a surgeon approaching lateral UKA, Fixed Bearing Metal-Backed design  
225 is preferable, given the lower failure rates and subsequently longer implant survivorship.

## 226 **Conclusion**

227 Considering actual evidence, for a surgeon approaching lateral UKA, the Fixed Bearing Metal-  
228 Backed design is preferable, given the lower failure rates and subsequently longer implant  
229 survivorship.

230

## 231 Bibliography

- 232 [1] Laskin RS. Unicompartamental knee replacement: some unanswered questions. *Clin Orthop*  
233 *Relat Res* 2001;267–71.
- 234 [2] Scott RD. Lateral unicompartamental replacement: a road less traveled. *Orthopedics*  
235 2005;28:983–4.
- 236 [3] Schindler OS, Scott WN, Scuderi GR. The practice of unicompartamental knee arthroplasty  
237 in the United Kingdom. *J Orthop Surg (Hong Kong)* 2010;18:312–9.  
238 <https://doi.org/10.1177/230949901001800311>.
- 239 [4] Lombardi AV, Berend KR, Walter CA, Aziz-Jacobo J, Cheney NA. Is recovery faster for  
240 mobile-bearing unicompartamental than total knee arthroplasty? *Clin Orthop Relat Res*  
241 2009;467:1450–7. <https://doi.org/10.1007/s11999-009-0731-z>.
- 242 [5] Smith TO, Chester R, Glasgow MM, Donell ST. Accelerated rehabilitation following  
243 Oxford unicompartamental knee arthroplasty: five-year results from an independent centre. *Eur J*  
244 *Orthop Surg Traumatol* 2012;22:151–8. <https://doi.org/10.1007/s00590-011-0797-7>.
- 245 [6] Laurencin CT, Zelicof SB, Scott RD, Ewald FC. Unicompartamental versus total knee  
246 arthroplasty in the same patient. A comparative study. *Clin Orthop Relat Res* 1991:151–6.
- 247 [7] Walker T, Gotterbarm T, Bruckner T, Merle C, Streit MR. Total versus unicompartamental  
248 knee replacement for isolated lateral osteoarthritis: a matched-pairs study. *Int Orthop*  
249 2014;38:2259–64. <https://doi.org/10.1007/s00264-014-2473-0>.
- 250 [8] Zuiderbaan HA, van der List JP, Khamaisy S, Nawabi DH, Thein R, Ishmael C, et al.  
251 Unicompartamental knee arthroplasty versus total knee arthroplasty: Which type of artificial joint do  
252 patients forget? *Knee Surg Sports Traumatol Arthrosc* 2017;25:681–6.  
253 <https://doi.org/10.1007/s00167-015-3868-1>.
- 254 [9] Isaac SM, Barker KL, Danial IN, Beard DJ, Dodd CA, Murray DW. Does arthroplasty type  
255 influence knee joint proprioception? A longitudinal prospective study comparing total and  
256 unicompartamental arthroplasty. *Knee* 2007;14:212–7. <https://doi.org/10.1016/j.knee.2007.01.001>.
- 257 [10] Ollivier M, Abdel MP, Parratte S, Argenson J-N. Lateral unicondylar knee arthroplasty  
258 (UKA): Contemporary indications, surgical technique, and results. *Int Orthop* 2014;38:449–55.  
259 <https://doi.org/10.1007/s00264-013-2222-9>.
- 260 [11] Fitzpatrick C, FitzPatrick D, Lee J, Auger D. Statistical design of unicompartamental tibial  
261 implants and comparison with current devices. *Knee* 2007;14:138–44.  
262 <https://doi.org/10.1016/j.knee.2006.11.005>.
- 263 [12] Gulati A, Chau R, Beard DJ, Price AJ, Gill HS, Murray DW. Localization of the full-  
264 thickness cartilage lesions in medial and lateral unicompartamental knee osteoarthritis. *J Orthop Res*  
265 2009;27:1339–46. <https://doi.org/10.1002/jor.20880>.
- 266 [13] Hamilton WG, Ammeen D, Engh CA, Engh GA. Learning Curve With Minimally Invasive  
267 Unicompartamental Knee Arthroplasty. *The Journal of Arthroplasty* 2010;25:735–40.  
268 <https://doi.org/10.1016/j.arth.2009.05.011>.
- 269 [14] Servien E, Merini A, Lustig S, Neyret P. Lateral uni-compartmental knee replacement:  
270 current concepts and future directions. *Knee Surg Sports Traumatol Arthrosc* 2013;21:2501–8.  
271 <https://doi.org/10.1007/s00167-013-2585-x>.
- 272 [15] Citak M, Cross MB, Gehrke T, Dersch K, Kendoff D. Modes of failure and revision of  
273 failed lateral unicompartamental knee arthroplasties. *Knee* 2015;22:338–40.  
274 <https://doi.org/10.1016/j.knee.2015.03.008>.
- 275 [16] Ernstbrunner L, Imam MA, Andronic O, Perz T, Wieser K, Fucentese SF. Lateral  
276 unicompartamental knee replacement: a systematic review of reasons for failure. *Int Orthop*  
277 2018;42:1827–33. <https://doi.org/10.1007/s00264-017-3662-4>.
- 278 [17] Moher D, Liberati A, Tetzlaff J, Altman DG, Group TP. Preferred Reporting Items for  
279 Systematic Reviews and Meta-Analyses: The PRISMA Statement. *PLOS Medicine*  
280 2009;6:e1000097. <https://doi.org/10.1371/journal.pmed.1000097>.

281 [18] Wright JG, Swiontkowski MF, Heckman JD. Introducing levels of evidence to the journal. *J*  
282 *Bone Joint Surg Am* 2003;85:1–3.

283 [19] Neyeloff JL, Fuchs SC, Moreira LB. Meta-analyses and Forest plots using a microsoft excel  
284 spreadsheet: step-by-step guide focusing on descriptive data analysis. *BMC Research Notes*  
285 2012;5:52. <https://doi.org/10.1186/1756-0500-5-52>.

286 [20] Mantel N, Haenszel W. Statistical aspects of the analysis of data from retrospective studies  
287 of disease. *J Natl Cancer Inst* 1959;22:719–48.

288 [21] Greenland S, Robins JM. Estimation of a common effect parameter from sparse follow-up  
289 data. *Biometrics* 1985;41:55–68.

290 [22] Higgins J, Thomas J, Chandler J, Cumpston M, Li T, Page M, et al. *Cochrane Handbook for*  
291 *Systematic Reviews of Interventions* version 6.2 (updated february 2021) Available from  
292 [www.training.cochrane.org/handbook](http://www.training.cochrane.org/handbook). Cochrane; 2021.

293 [23] Lustig S, Elguindy A, Servien E, Fary C, Munini E, Demey G, et al. 5- to 16-year follow-up  
294 of 54 consecutive lateral unicondylar knee arthroplasties with a fixed-all polyethylene bearing. *J*  
295 *Arthroplasty* 2011;26:1318–25. <https://doi.org/10.1016/j.arth.2011.01.015>.

296 [24] Berend KR, Kolczun MC, George JW, Lombardi AV. Lateral Unicompartmental Knee  
297 Arthroplasty Through a Lateral Parapatellar Approach Has High Early Survivorship. *Clin Orthop*  
298 *Relat Res* 2012;470:77–83. <https://doi.org/10.1007/s11999-011-2005-9>.

299 [25] Streit MR, Walker T, Bruckner T, Merle C, Kretzer JP, Clarius M, et al. Mobile-bearing  
300 lateral unicompartmental knee replacement with the Oxford domed tibial component: an  
301 independent series. *J Bone Joint Surg Br* 2012;94:1356–61. [https://doi.org/10.1302/0301-](https://doi.org/10.1302/0301-620X.94B10.29119)  
302 [620X.94B10.29119](https://doi.org/10.1302/0301-620X.94B10.29119).

303 [26] Altuntas AO, Alsop H, Cobb JP. Early results of a domed tibia, mobile bearing lateral  
304 unicompartmental knee arthroplasty from an independent centre. *Knee* 2013;20:466–70.  
305 <https://doi.org/10.1016/j.knee.2012.11.008>.

306 [27] Liebs TR, Herzberg W. Better quality of life after medial versus lateral unicondylar knee  
307 arthroplasty. *Clin Orthop Relat Res* 2013;471:2629–40. <https://doi.org/10.1007/s11999-013-2966-y>.

308 [28] Lustig S, Lording T, Frank F, Debette C, Servien E, Neyret P. Progression of medial  
309 osteoarthritis and long term results of lateral unicompartmental arthroplasty: 10 to 18 year follow-  
310 up of 54 consecutive implants. *Knee* 2014;21 Suppl 1:S26-32. [https://doi.org/10.1016/S0968-](https://doi.org/10.1016/S0968-0160(14)50006-3)  
311 [0160\(14\)50006-3](https://doi.org/10.1016/S0968-0160(14)50006-3).

312 [29] Smith JRA, Robinson JR, Porteous AJ, Murray JRD, Hassaballa MA, Artz N, et al. Fixed  
313 bearing lateral unicompartmental knee arthroplasty--short to midterm survivorship and knee scores  
314 for 101 prostheses. *Knee* 2014;21:843–7. <https://doi.org/10.1016/j.knee.2014.04.003>.

315 [30] Weston-Simons JS, Pandit H, Kendrick BJL, Jenkins C, Barker K, Dodd C a. F, et al. The  
316 mid-term outcomes of the Oxford Domed Lateral unicompartmental knee replacement. *Bone Joint J*  
317 2014;96-B:59–64. <https://doi.org/10.1302/0301-620X.96B1.31630>.

318 [31] Demange MK, Von Keudell A, Probst C, Yoshioka H, Gomoll AH. Patient-specific  
319 implants for lateral unicompartmental knee arthroplasty. *Int Orthop* 2015;39:1519–26.  
320 <https://doi.org/10.1007/s00264-015-2678-x>.

321 [32] Kim KT, Lee S, Kim J, Kim JW, Kang MS. Clinical Results of Lateral Unicompartmental  
322 Knee Arthroplasty: Minimum 2-Year Follow-up. *Clin Orthop Surg* 2016;8:386–92.  
323 <https://doi.org/10.4055/cios.2016.8.4.386>.

324 [33] Edmiston TA, Manista GC, Courtney PM, Sporer SM, Della Valle CJ, Levine BR. Clinical  
325 Outcomes and Survivorship of Lateral Unicompartmental Knee Arthroplasty: Does Surgical  
326 Approach Matter? *J Arthroplasty* 2018;33:362–5. <https://doi.org/10.1016/j.arth.2017.09.009>.

327 [34] Newman SDS, Altuntas A, Alsop H, Cobb JP. Up to 10 year follow-up of the Oxford  
328 Domed Lateral Partial Knee Replacement from an independent centre. *Knee* 2017;24:1414–21.  
329 <https://doi.org/10.1016/j.knee.2017.05.001>.

330 [35] Fornell S, Prada E, Barrena P, García-Mendoza A, Borrego E, Domecq G. Mid-term  
331 outcomes of mobile-bearing lateral unicompartmental knee arthroplasty. *Knee* 2018;25:1206–13.

332 <https://doi.org/10.1016/j.knee.2018.05.016>.

333 [36] Walker T, Zahn N, Bruckner T, Streit MR, Mohr G, Aldinger PR, et al. Mid-term results of  
334 lateral unicondylar mobile bearing knee arthroplasty: a multicentre study of 363 cases. *Bone Joint J*  
335 2018;100-B:42–9. <https://doi.org/10.1302/0301-620X.100B1.BJJ-2017-0600.R1>.

336 [37] Deroche E, Batailler C, Lording T, Neyret P, Servien E, Lustig S. High Survival Rate and  
337 Very Low Wear of Lateral Unicompartmental Arthroplasty at Long Term: A Case Series of 54  
338 Cases at a Mean Follow-Up of 17 Years. *J Arthroplasty* 2019;34:1097–104.  
339 <https://doi.org/10.1016/j.arth.2019.01.053>.

340 [38] Zambianchi F, Franceschi G, Rivi E, Banchelli F, Marcovigi A, Khabbazzè C, et al. Clinical  
341 results and short-term survivorship of robotic-arm-assisted medial and lateral unicompartmental  
342 knee arthroplasty. *Knee Surg Sports Traumatol Arthrosc* 2020;28:1551–9.  
343 <https://doi.org/10.1007/s00167-019-05566-4>.

344 [39] Burger JA, Kleeblad LJ, Laas N, Pearle AD. Mid-term survivorship and patient-reported  
345 outcomes of robotic-arm assisted partial knee arthroplasty. *Bone Joint J* 2020;102-B:108–16.  
346 <https://doi.org/10.1302/0301-620X.102B1.BJJ-2019-0510.R1>.

347 [40] Kennedy JA, Mohammad HR, Yang I, Mellon SJ, Dodd CAF, Pandit HG, et al. Oxford  
348 domed lateral unicompartmental knee arthroplasty. *Bone Joint J* 2020;102-B:1033–40.  
349 <https://doi.org/10.1302/0301-620X.102B8.BJJ-2019-1330.R2>.

350 [41] Mohammad HR, Matharu GS, Judge A, Murray DW. The Mid- to Long-Term Outcomes of  
351 the Lateral Domed Oxford Unicompartmental Knee Replacement: An Analysis From the National  
352 Joint Registry for England, Wales, Northern Ireland, and the Isle of Man. *J Arthroplasty*  
353 2021;36:107–11. <https://doi.org/10.1016/j.arth.2020.07.031>.

354 [42] Tu Y, Ma T, Wen T, Yang T, Xue L, Xue H. Does Unicompartmental Knee Replacement  
355 Offer Improved Clinical Advantages Over Total Knee Replacement in the Treatment of Isolated  
356 Lateral Osteoarthritis? A Matched Cohort Analysis From an Independent Center. *J Arthroplasty*  
357 2020;35:2016–21. <https://doi.org/10.1016/j.arth.2020.03.021>.

358 [43] Xue H, Ma T, Wen T, Yang T, Xue L, Tu Y. Predictors of Satisfactory Outcomes With  
359 Fixed-Bearing Lateral Unicompartmental Knee Arthroplasty: Up to 7-year Follow-Up. *J*  
360 *Arthroplasty* 2021;36:910–6. <https://doi.org/10.1016/j.arth.2020.10.001>.

361 [44] Abu Al-Rub Z, Lamb JN, West RM, Yang X, Hu Y, Pandit HG. Survivorship of fixed vs  
362 mobile bearing unicompartmental knee replacement: A systematic review and meta-analysis of  
363 sixty-four studies and National Joint Registries. *Knee* 2020;27:1635–44.  
364 <https://doi.org/10.1016/j.knee.2020.09.004>.

365 [45] Burger JA, Kleeblad LJ, Sierevelt IN, Horstmann WG, Nolte PA. Bearing design influences  
366 short- to mid-term survivorship, but not functional outcomes following lateral unicompartmental  
367 knee arthroplasty: a systematic review. *Knee Surg Sports Traumatol Arthrosc* 2019;27:2276–88.  
368 <https://doi.org/10.1007/s00167-019-05357-x>.

369 [46] Burger JA, Kleeblad LJ, Sierevelt IN, Horstmann WG, van Geenen RCI, van Steenbergen  
370 LN, et al. A Comprehensive Evaluation of Lateral Unicompartmental Knee Arthroplasty Short to  
371 Mid-Term Survivorship, and the Effect of Patient and Implant Characteristics: An Analysis of Data  
372 From the Dutch Arthroplasty Register. *J Arthroplasty* 2020;35:1813–8.  
373 <https://doi.org/10.1016/j.arth.2020.02.027>.

374 [47] Scott CEH, Nutton RW, Biant LC. Lateral compartment osteoarthritis of the knee:  
375 Biomechanics and surgical management of end-stage disease. *Bone Joint J* 2013;95-B:436–44.  
376 <https://doi.org/10.1302/0301-620X.95B4.30536>.


377 [48] James EW, LaPrade CM, LaPrade RF. Anatomy and biomechanics of the lateral side of the  
378 knee and surgical implications. *Sports Med Arthrosc Rev* 2015;23:2–9.  
379 <https://doi.org/10.1097/JSA.0000000000000040>.

380 [49] Schelfaut S, Beckers L, Verdonk P, Bellemans J, Victor J. The risk of bearing dislocation in  
381 lateral unicompartmental knee arthroplasty using a mobile biconcave design. *Knee Surg Sports*  
382 *Traumatol Arthrosc* 2013;21:2487–94. <https://doi.org/10.1007/s00167-012-2171-7>.


383 [50] Kendrick BJL, Simpson DJ, Kaptein BL, Valstar ER, Gill HS, Murray DW, et al.  
384 Polyethylene wear of mobile-bearing unicompartmental knee replacement at 20 years. *J Bone Joint*  
385 *Surg Br* 2011;93:470–5. <https://doi.org/10.1302/0301-620X.93B4.25605>.  
386 [51] van der List JP, Kleeblad LJ, Zuiderbaan HA, Pearle AD. Mid-Term Outcomes of Metal-  
387 Backed Unicompartmental Knee Arthroplasty Show Superiority to All-Polyethylene  
388 Unicompartmental and Total Knee Arthroplasty. *HSS J* 2017;13:232–40.  
389 <https://doi.org/10.1007/s11420-017-9557-5>.  
390 [52] Koh IJ, Suhl KH, Kim MW, Kim MS, Choi KY, In Y. Use of All-polyethylene Tibial  
391 Components in Unicompartmental Knee Arthroplasty Increases the Risk of Early Failure. *J Knee*  
392 *Surg* 2017;30:807–15. <https://doi.org/10.1055/s-0036-1597979>.  
393 [53] Swienckowski JJ, Pennington DW. Unicompartmental knee arthroplasty in patients sixty  
394 years of age or younger. *J Bone Joint Surg Am* 2004;86-A Suppl 1:131–42.  
395 <https://doi.org/10.2106/00004623-200409001-00004>.  
396 [54] Sah AP, Scott RD. Lateral unicompartmental knee arthroplasty through a medial approach.  
397 Study with an average five-year follow-up. *J Bone Joint Surg Am* 2007;89:1948–54.  
398 <https://doi.org/10.2106/JBJS.F.01457>.  
399 [55] Gunther TV, Murray DW, Miller R, Wallace DA, Carr AJ, O'Connor JJ, et al. Lateral  
400 unicompartmental arthroplasty with the Oxford meniscal knee. *The Knee* 1996;3:33–9.  
401 [https://doi.org/10.1016/0968-0160\(96\)00208-6](https://doi.org/10.1016/0968-0160(96)00208-6).  
402 [56] Argenson J-NA, Komistek RD, Aubaniac J-M, Dennis DA, Northcut EJ, Anderson DT, et  
403 al. In vivo determination of knee kinematics for subjects implanted with a unicompartmental  
404 arthroplasty. *J Arthroplasty* 2002;17:1049–54. <https://doi.org/10.1054/arth.2002.34527>.  
405 [57] Han S-B, Lee S-S, Kim K-H, Im J-T, Park P-S, Shin Y-S. Survival of medial versus lateral  
406 unicompartmental knee arthroplasty: A meta-analysis. *PLoS One* 2020;15:e0228150.  
407 <https://doi.org/10.1371/journal.pone.0228150>.  
408

409

411

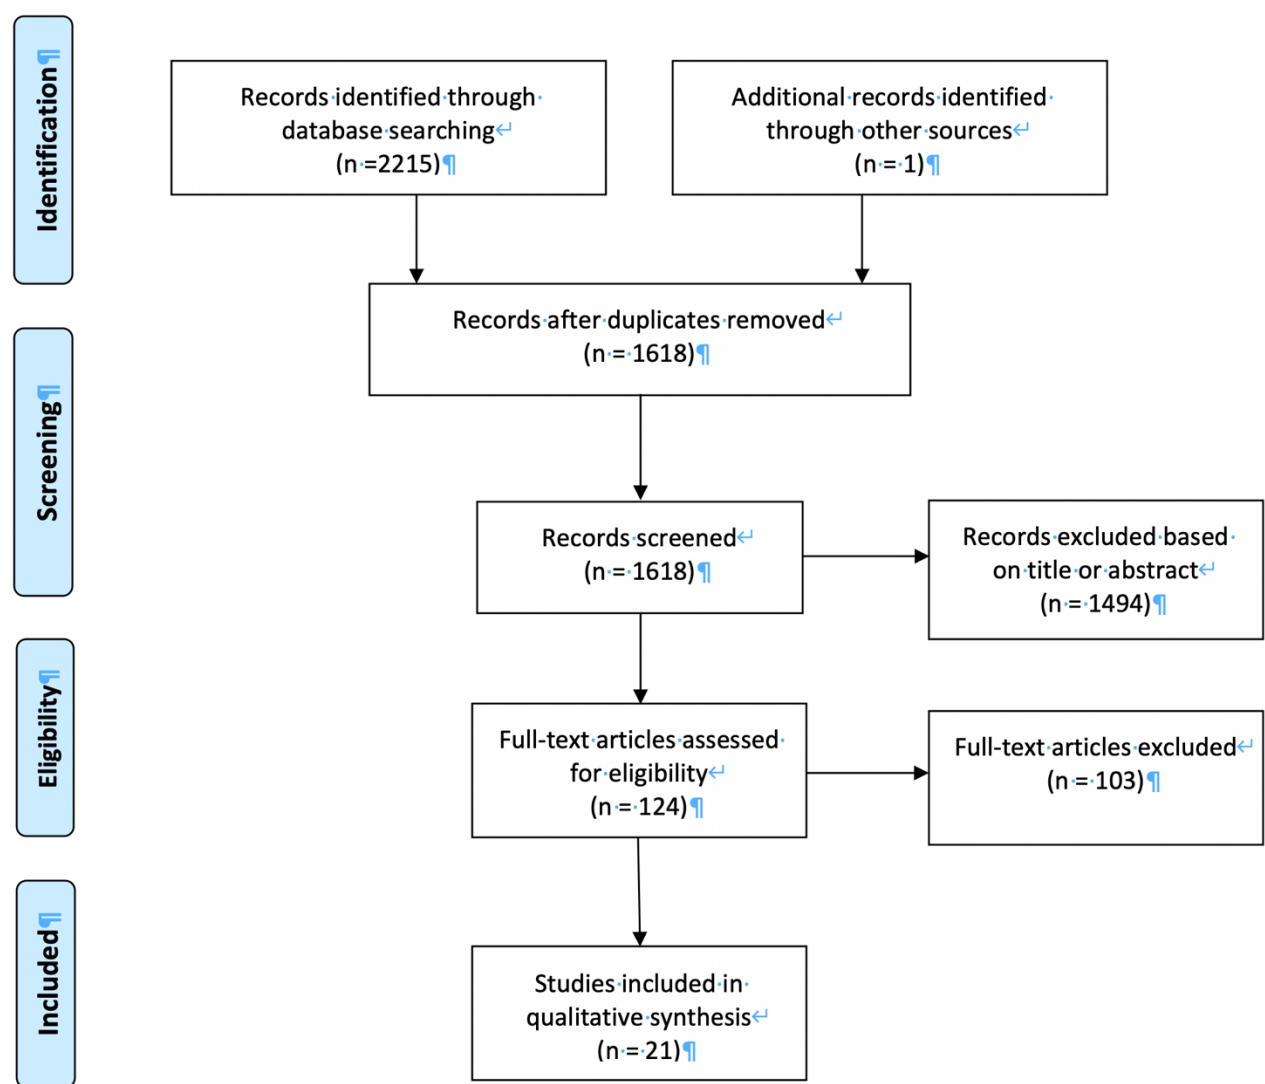

412   **Fig.1** Overview of screening and selection process for the systematic review.

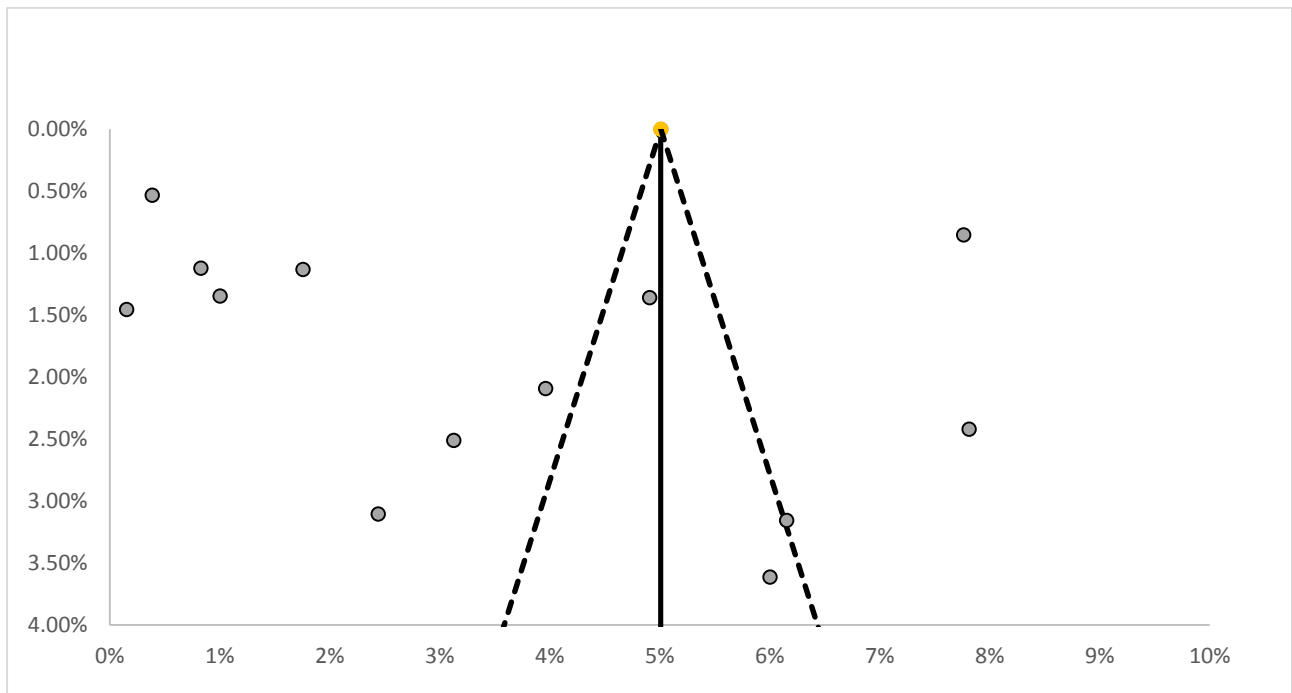

413

414

415

416

**Fig. 2** Funnel plot assessing potential publication bias from failure rates. Thirteen studies were analyzed, the abscissa axis showed the failure rates, and the vertical axis showed the standard error.




Author	Year	LOE	Type of Study	No. Of Patients (Knees)	Age, Mean $\pm$ SD (Range), y	Male Sex, n (%)	Type of Implant	Implant	Follow-up, Mean $\pm$ SD (Range), y	Quality score (mCS)
Burger et al.	2020	IV	Retrospective	NA (171)	64.4 $\pm$ 11 (NA)	69 (40.4)	FB M-B	Stryker Restoris MCK	4.3 $\pm$ 1.7 (NA)	65
Kennedy et al.	2020	II	Prospective	300 (325)	64.9 $\pm$ 11 (39-90)	96 (37)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	7 $\pm$ 2,7 (3-14)	70
Mohammad et al.	2020	II	Retrospective	NA (992)	64.5 $\pm$ 12,5 (NA)	351 (35.4)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	5 $\pm$ 3.0 (NA)	41
Tu et al.	2020	II	Prospective	121 (121)	70.2 $\pm$ 8.8 (NA)	38 (31.4)	FB M-B	Waldemar Link Sled UKA	5.3 $\pm$ 2.5 (2-12.4)	84
Xue et al.	2020	IV	Retrospective	248 (260)	70.6 $\pm$ 8.5 (NA)	56 (28.3)	FB M-B	Waldemar Link Sled UKA	4.7 $\pm$ 1.1 (NA)	61
Deroche et al.	2019	IV	Retrospective	52 (54)	65.4 $\pm$ 11 (25-79)	6 (15.4)	FB A-P	NA, two different implants	17.9 $\pm$ 2 (15-23)	66
Zambianchi et al.	2019	IV	Retrospective	66 (67)	62.1 $\pm$ 9.5 (NA)	16 (24.2%)	FB M-B	Stryker Restoris MCK	3.0 $\pm$ NA (NA)	51
Fornell et al.	2018	IV	Retrospective	41 (41)	63 $\pm$ 10.8 (38-81)	10 (24.4)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	4.1 $\pm$ 1.2 (2.1-7)	62
Walker et al.	2018	IV	Retrospective	327 (344)	65 $\pm$ 13 (36-88)	90 (27.5)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	3.1 $\pm$ 1.7 (1-7.8)	64
Edmiston et al.	2017	IV	Retrospective	65 (65)	61.3 $\pm$ 11.2 (NA)	22 (34)	FB M-B	Zimmer Unicompartmental High Flex Knee, Zimmer Miller-Galante Unicompartmental Knee	6.6 $\pm$ 3.1 (NA)	48
Newman et al.	2017	IV	Retrospective	58 (64)	71 $\pm$ 12 (44-92)	17 (29.3)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	6.7 $\pm$ 2.0 (2-9.9)	72
Kim et al.	2016	IV	Retrospective	27 (30)	63.3 $\pm$ 8 (48-80)	15 (50)	FB M-B	Zimmer Unicompartmental High Flex Knee	3.2 $\pm$ 0.5 (2-4)	61
Demange et al.	2015	IV	Retrospective	32 (33)	57.5 $\pm$ 8.9 (36-88)	20 (39.2)	FB M-B	ConforMIS iUni G1 (1st gen) Zimmer Miller-Galante Unicompartmental Knee	4.7 $\pm$ 1.2 (2-9.1)	66
Lustig et al.	2014	IV	Retrospective	52 (54)	72.2 $\pm$ 15.2 (25-85)	7 (15.9)	FB A-P	Tornier HLS Uni Evolution	14.2 $\pm$ 1.95 (10.2-18)	66
Smith et al.	2014	IV	Retrospective	100 (101)	64.8 $\pm$ 13.8 (36-91)	32 (32)	FB A-P	Corin AMC Uniglide	5.0 $\pm$ 0.0 (5-5)	82
Weston-Simons et al.	2014	II	Prospective	258 (265)	64 $\pm$ 14.5 (32-90)	91 (35.3)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	4.0 $\pm$ 2.2 (0.5-8.3)	72
Altuntas et al.	2013	IV	Retrospective	58 (64)	71 $\pm$ 12 (44-92)	17 (29.3)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	3.2 $\pm$ 0.8 (2-5.1)	59
Liebs et al.	2013	IV	Retrospective	128 (128)	73.6 $\pm$ 11.8 (44-91)	NA (33)	MB M-B	DePuy Preservation UKA	6.0 $\pm$ 1.9 (2.1-9.8)	75
Berend et al.	2012	IV	Retrospective	97 (100)	68.8 $\pm$ 14 (NA)	38 (30)	FB M-B	Biomet Respicci II UKA Biomet Vanguard M UKA	3.3 $\pm$ 1.2 (2-6.8)	59
Streit et al.	2012	II	Prospective	50 (50)	60 $\pm$ 11.3 (36-81)	20 (40)	MB M-B	Zimmer Biomet Oxford Doomed Lateral UKR	3 $\pm$ 0.6 (2-4.3)	71
Lustig et al.	2011	IV	Retrospective	47 (49)	72.2 $\pm$ 3 (25-88)	8 (17)	FB A-P	Tornier HLS Uni Evolution	8.4 $\pm$ 2.6 (5.3-15.8)	60

417 **Tab. 1** Study characteristics and patients demographics. FB, Fixed Bearing; MB, Mobile Bearing; A-P, All Polyethylene; M-B, Metal Backed; NA, Non Available

	Failure Rate	95% CI Lower Limit	95%CI Upper Limit
FB A-P	8,6%	3,2%	14,1%
FB M-B	0,8%	0,0%	1,6%
MB M-B	7,1%	5,3%	8,9%
All	5,0%	3,1%	6,9%

**Tab. 2** Failure rates by implant design

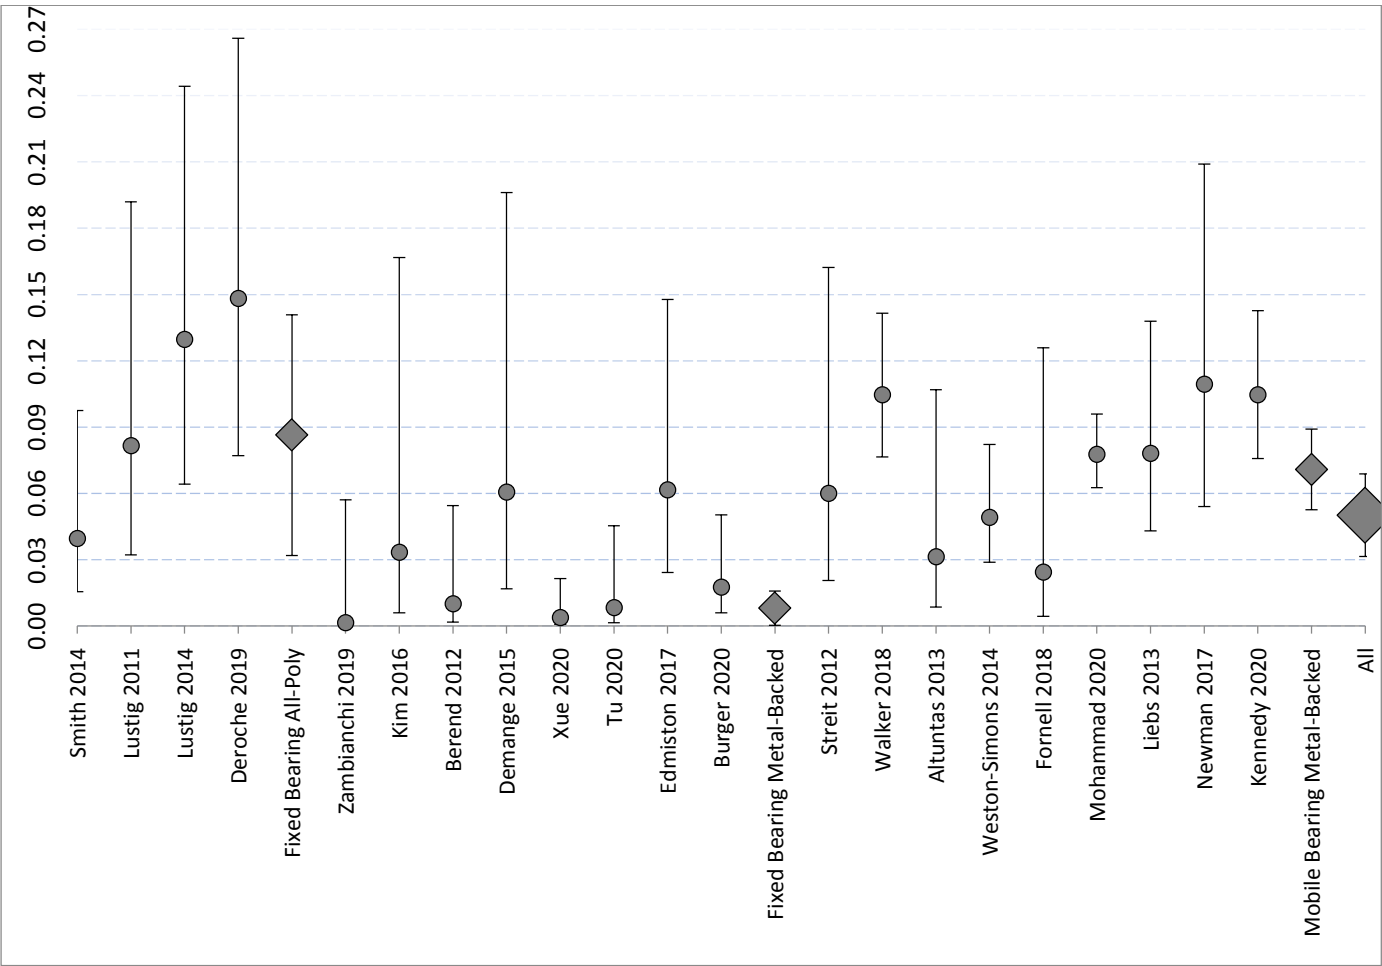

**Fig. 3** Results of aggregate analysis for comparison of failure rates between patients with FB A-P, FB M-B and MB M-B implants. Y-axis shows failure rate, X-axis shows examined studies.

Implant design (comparison)	Mean Failure Rate	95% CI Lower Limit	95% CI Upper Limit	p-value
FB A-P	9%	3%	14%	0,024
FB F-B	1%	0%	2%	
FB A-P	9%	3%	14%	>0,999
MB M-B	7%	5%	9%	
FB M-B	1%	0%	2%	0,000
MB M-B	7%	5%	9%	


425 **Tab. 3** Comparison of failure rates among groups by implant designs.

426

	Failure Rate	95% CI Lower Limit	95%CI Upper Limit
FU < 5y	3,9%	1,6%	6,3%
5y <FU < 10y	7,0%	2,6%	11,4%
FU > 10y	8,9%	0,0%	18,7%
All	5,0%	3,1%	6,9%

427 **Tab. 4** Failure rates by follow-up time

428

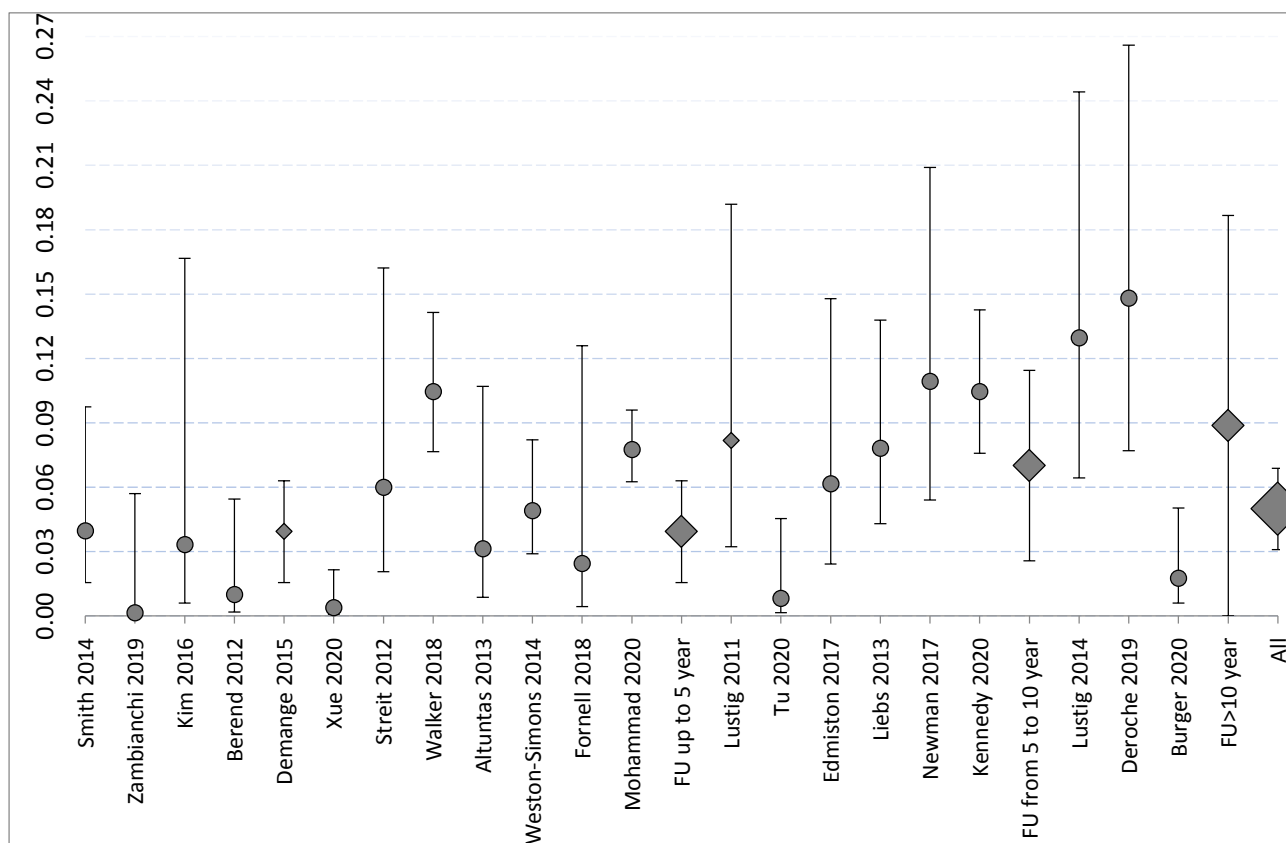

**Fig. 4** Results of aggregate analysis for comparison of failure rates between patients with a follow-up less than 5 years, between 5 and 10 years, and more than 10 years. Y-axis shows failure rate, X-axis shows examined studies.

Follow-up (comparison)	Mean Failure Rate	95% CI Lower Limit	95% CI Upper Limit	p-value
FU < 5y	4%	2%	6%	0,582
5y < FU < 10y	7%	3%	11%	
FU < 5y	4%	2%	6%	0,754
FU > 10y	9%	0%	19%	
5y < FU < 10y	7%	3%	11%	>0,999
FU > 10y	9%	0%	19%	

**Tab. 5** Comparison of failure rates among groups by follow-up time.

Author	Reoperations	Failure, n (%)	Survivorship
Lustig 2011	4 cases were revised 1 TKA	NA	98.08% at 10 years; end-point removal of the prosthesis
Berend 2012	3 revisions for UKA in the medial compartment 3 patients had reoperations 1 ORIF for fracture 1 arthroscopy for a medial meniscal tear	NA	NA
Streit 2012	1TKA revision for pain 3 patients had revision 2 TKA due to dislocation	3 cases (6.2%) Dislocation at 3 years.	94% at 3 years, end-point revision for any reason
Altuntas 2013	1 TKA due to MRSA infection 4 patients had reoperation 2 had re-operations unrelated to the implant 2 required revision of prosthesis [Instability (1); Medial OA (1)]	3.1% failure rate of prosthesis no case of bearing dislocation	97% at 38 months; end point revision of implant
Liebs 2013	14 patient had revision 6 Aseptic loosening 2 Medial OA 2 Fracture 1 Patellofemoral pain 1 Internal fixation with screws, no change of implant components 1 Impingement	NA	83% at 9 years; end-point prosthesis survival
Lustig 2014	1 Arthroscopy, without change of components 7 patient had undergone a second operation 3 were revised to TKA 3 had medial UKAs for medial OA 1 TKA for tibial tray malpositioning	NA	91.4% at 15 years ,end-point removal of the prosthesis
Smith 2014	4 knees had revision 1 Medial OA 1 Tibial loosening 1 Infection 1 Unknown	NA	95.5% at 5 year; end-point removal of the prosthesis
Weston-Simons 2014	13 knees (4.9%) had re-operations 4 dislocation 3 Medial OA 3 Infection 3 Ongoing pain	NA	92.1% at 8 years; end point any revision
Demange 2015	In custom implant group 2 revision 1 infection so two-stage re-implantation with custom implant 1 prosthesis failure so TKA In the standard implant group, 3 implants failed 1 Infection 2 progression of disease Revision to TKA in 1 case due to ongoing pain	NA	97% at average 37 months, in custom implant group 85% at an average of 33 months in the standard implant group
Kim 2016	Revision to TKA in 1 case due to ongoing pain	3.3 % failure rate of prosthesis	96.7% at 38 months, end point removal of prosthesis
Edmiston 2017	4 patient had revision surgery 1 ongoing pain 1 posttraumatic wound dehiscence 1 medial OA 1 patellofemoral arthritis	5% failure in in lateral approach 7% failure in medial approach	94% at a mean of 82 months; end point revision surgery
Newman 2017	2 patient revised into TKA (1 Medial OA, 1 ongoing pain) 6 patient had further surgery without prosthesis removal 1 exchange of bearing due to instability 1 arthroscopic lavage for haematoma 1 ACL reconstruction with bearing exchange 2 medial UKRs for medial OA 1 exchange of bearing due to instability	7% knee revised 13% was reoperation rate	87% at 80.6 months; end point re-operation
Fornell 2018	1 patient revised to TKA due to ongoing pain 1 arthroscopic reduction of dislocation	2.4% revision 2.4% dislocation	97.5% at 5 years; endpoint revision for any reason
Walker 2018	36 knees had revision surgery (in 6 patient more than 1 procedure) 3 infection 20 dislocation (19 revised while 1 had spontaneous repositioning) 18 patients revised into TKA (5 dislocation, 6 medial OA, 3 instability, 3 ongoing pain, 1 femoral component loosening)	10.5 % revision 8.5 % dislocation	85.0% at 5 years; end point revision surgery
Deroche 2019	8 knees had revision 3 medial uka for medial OA 4 TKA for medial and symptomatic patellofemoral OA	20.5 % revision	82.1% at 15 years and 79.4% at 20 years end point prosthesis removal and/or a second UKA for OA
Burger 2020	1TKA for aseptic loosening of the tibial component 3 revision to TKA 1 infection 1 Aseptic loosening 1 ongoing pain	NA	97.7% at 5 Year; end point revision surgery
Zambianchi 2019	Arthroscopy performed in 2 cases 1 for medial meniscus tear 1 for synovitis in medial cpmartment Radiological outcome was not reported	No revisions	100% at 3 years; revision as the endpoint 96.9% (CI 88.0–99.2%) at 3 years; reoperation as the endpoint
Kennedy 2020	7 bearing exchange alone 7 bearing exchange with screw augmentation	34 (10%) revisions 14 knees bearing dislocation	92.1% at 5 year; end-point revision for any reason 84.6% at 10 years, end-point revision for any reason

	1 bearing exchange with debridement 1 bearing exchange with exploration for pain 1 bearing exchange with femoral component revision 11 single-stage TKA 5 addition of medial uKa 1 conversion to a fixed bearing tibial component 1 two-stage TKA Radiological outcome was not reported	12 knees progression of osteoarthritis 1 aseptic femoral loosening 1 deep infection 2 recurrent haemarthrosis 1 unrelated patellar fracture 3 bearing exchanged	
<b>Mohammad 2020</b>	NA	77 knees (7.8%) revision surgery	92.4% (CI: 90.3-94.1) at 5 year; endpoint any revision surgery 88.6% (CI: 85.3-91.2) at 10 year; endpoint any revision surgery
	Radiological outcome was not reported	23 Dislocation subluxation revision	96.0% (CI: 91.4-98.2) at 5 year for normal weight
		15 Pain	92.3% (CI: 88.3-95.0) at 5 year for overweight
		14 Aseptic loosening	89.7% (CI: 84.8-93.1) at 5 year for obese
		12 OA progression	
		6 Component dissociation	86.0% (CI: 80.2-90.3) at 5 year for <55 year
		6 Infection	92.9% (CI: 88.4-95.7) at 5 year for 55-64 years
		3 Instability	94.9% (CI: 91.3-97.1) at 5 year for 65-74 year
		1 Periprosthetic fracture	95.6% (CI: 91.1-97.8) at 5 year for 75 and more
		1 Lysis	
		1 Wear	
		1 Stiffness	
		14 others	
<b>Tu 2020</b>	1 medial UKA for medial OA	NA	99.2%, at 5 years; revision for any reason as the end point
<b>Xue 2020</b>	1 medial UKA for medial OA	NA	99.5% at 5 years; endpoint revision of prosthesis

## Reoperations and failures overview