

Chemiluminescence-based biosensor for monitoring astronauts' health status during space missions: results from the International Space Station (ISS)

Martina Zangheri¹, Mara Mirasoli¹, Massimo Guardigli¹, Fabio Di Nardo², Laura Anfossi², Claudio Baggiani², Patrizia Simoni³, Mario Benassai⁴, Aldo Roda^{1*}

1. Department of Chemistry "Giacomo Ciamician", Alma Mater Studiorum – University of Bologna, Via Selmi 2, 40126 Bologna, Italy
2. Department of Chemistry, University of Turin, Via Pietro Giuria, 7, 10125 Turin, Italy
3. Department of Medical and Surgical Sciences, Alma Mater Studiorum – University of Bologna, Via Massarenti 9, 40138 Bologna, Italy
4. Altec SpA, Corso Marche 79, 10146 Torino, Italy

*Corresponding author

Prof. Aldo Roda

Department of Chemistry "Giacomo Ciamician", Alma Mater Studiorum - University of Bologna

via Selmi 2, 40126 Bologna, Italy

Tel/fax +39 051 343398

E-mail aldo.roda@unibo.it

Supplementary material

2. Materials and methods

2.3 Buffers for cortisol-HRP conjugate working solution

Composition of buffers tested to achieve long-term stability of cortisol-HRP conjugate working solution.

- Buffer A: 100 mmol L⁻¹ 2-(N-morpholino)ethanesulfonic acid (MES), 1 mmol L⁻¹ ethylenediaminetetraacetic acid (EDTA), 1 mmol L⁻¹ MgCl₂, 0.01% Thimerosal, 0.1% streptomycin sulfate, 1 mmol L⁻¹ SrCl₂, 1:1000 Proclin 300, 0.1% gum arabic, 3% BSA, 0.1% Tween 20, pH 6.0.
- Buffer B: 16 mmol L⁻¹ Na₂HPO₄, 4 mmol L⁻¹ NaH₂PO₄, 1 mmol L⁻¹ EDTA, 1 mmol L⁻¹ MgCl₂, 1 mmol L⁻¹ SrCl₂, 0.1% streptomycin sulphate, 0.1% Proclin 300, 0.1%, Gum Arabic, 3% BSA, 0.1% Tween 20, pH 7.4.
- Buffer C: 25 mmol L⁻¹ Na₂HPO₄, 75 mmol L⁻¹ NaH₂PO₄, 0.015% 8-anilino-1-naphthalenesulfonic acid, 3% BSA, 0.1% Tween 20, pH 6.5.
- Buffer D: 100 mmol L⁻¹ 2-(N-morpholino)ethanesulfonic acid (MES), 1 mmol L⁻¹ EDTA, 1 mmol L⁻¹ MgCl₂, 0.1% streptomycin sulfate, 1 mmol L⁻¹ SrCl₂, 10 μmol L⁻¹ hemin, 50 mg L⁻¹ cytochrome c, 1:1000 Proclin 300, 0.1% gum arabic, 3% BSA, 0.1% Tween 20, pH 6.0.
- Buffer E: 50 mmol L⁻¹ boric acid, 50 mmol L⁻¹ sodium citrate, 0.1% BSA, 0.05% Tween 20, 0.01% thimerosal, 8 mmol L⁻¹ EDTA, pH 6.0.

3. Results and discussion

3.1 Optimization of the immunoassay

3.1.1 Anti-cortisol antibody

The anti-cortisol antibody selected for LFIA development was immobilized at different dilutions (ranging from 1:500 to 1:10,000 v/v) on LFIA nitrocellulose membranes, then tested by analysing cortisol-free oral fluid samples and cortisol-spiked (1 and 10 ng mL⁻¹) oral fluid samples. Results are shown in Figure S1.

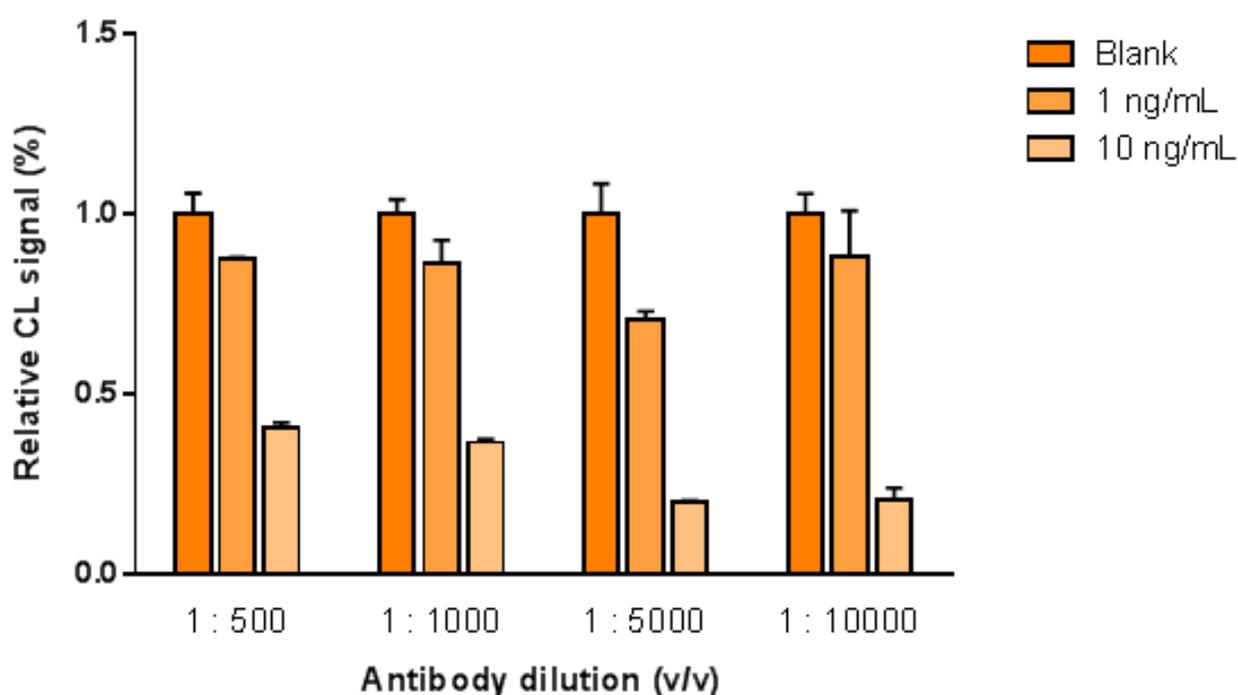


Figure S1: CL signals obtained upon immobilizing anti-cortisol antibody at different concentrations on LFIA nitrocellulose membranes and then analysing oral fluid samples at different cortisol concentrations (0, 1 and 10 ng mL⁻¹). Results are normalized for the signal obtained in the absence of cortisol.

3.1.4 LFIA strip materials

Different commercial sample pads were tested by analysing cortisol-free oral fluid samples. As shown in Figure S2, the highest signal/background ratio was obtained using the saliva pad II, which was thus selected for assay development.

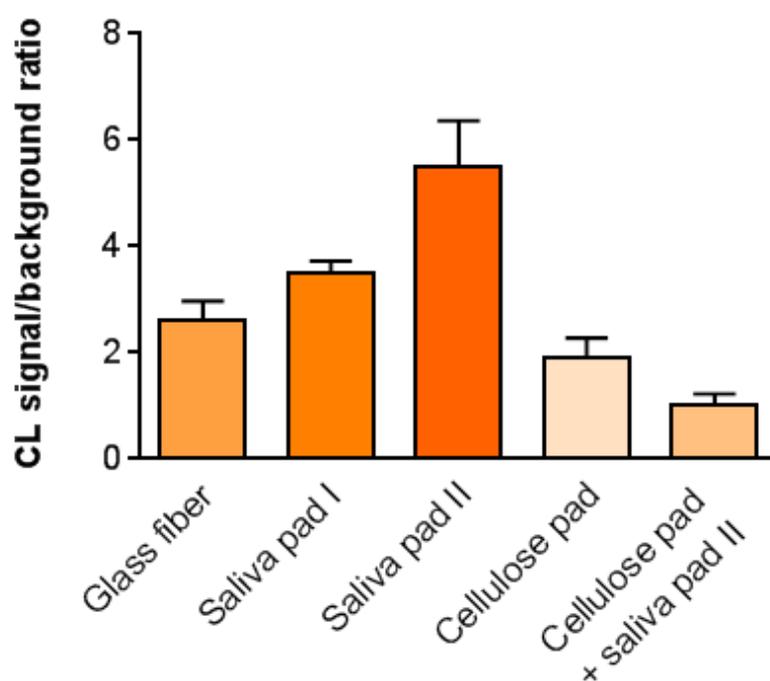


Figure S2: CL signals/background ratio values obtained upon analysing cortisol-free oral fluid samples on LFIA strips equipped with different commercial sample pads.

3.1.5 Shelf-life of reagents: stability of HRP-cortisol conjugate

Different conservation buffers (A - E) were evaluated by performing an accelerated storage test on cortisol-HRP conjugate solutions at three concentration levels, namely 1:250, 1:500 and 1:1000 (v/v) dilutions.

As shown in Figure S3, buffers D and E provided a satisfactory stability of cortisol-HRP conjugate (up to 3 weeks at 37°C) at all concentration levels, while buffers A, B and C buffers were not able to preserve its activity.

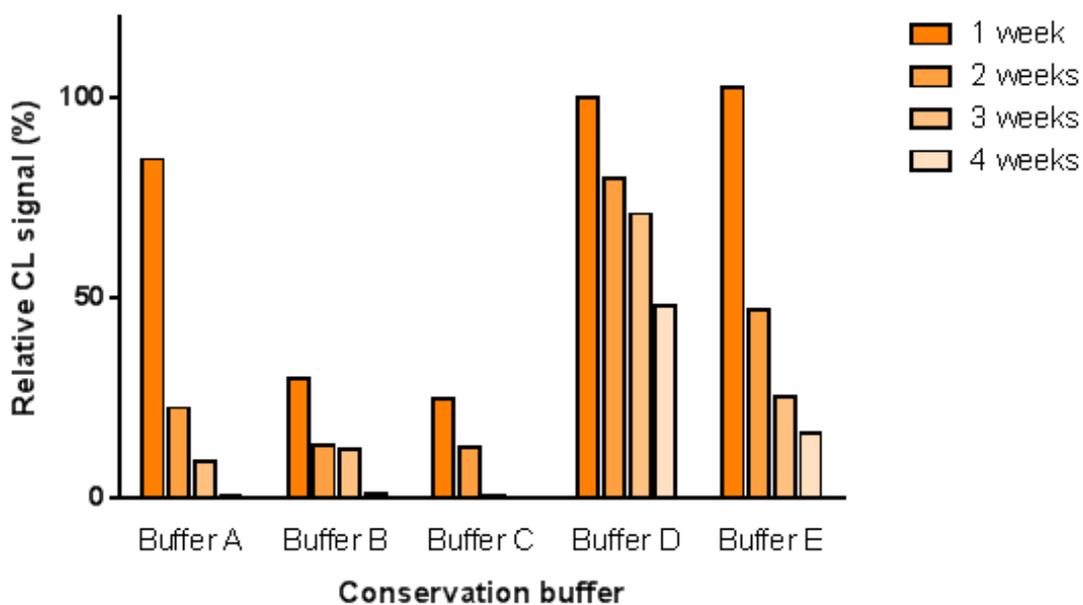


Figure S3: CL signals obtained upon analysing cortisol-free oral fluid samples employing cortisol-HRP conjugate solutions prepared at three concentration levels (1:250, 1:500 and 1:1000 (v/v) dilutions) in different conservation buffers (A - E) and stored at 37°C for up to 4 weeks. Results are compared with those obtained using a freshly prepared cortisol-HRP conjugate solution in the same buffer.

3.1.6 Washing

To eliminate the washing step prior to CL measurement we evaluated the possibility to increase the amount of CL substrate loaded onto the LFIA strip and exploit the flow of the CL substrate also for washing.

As shown in Figure S4, both washing of the LFIA strip with PBS (50 μ l) prior to the CL measurement and increase up to 70 μ l of the amount of the CL substrate loaded in the sample pad eliminated the interference of the oral fluid matrix on the CL reaction.

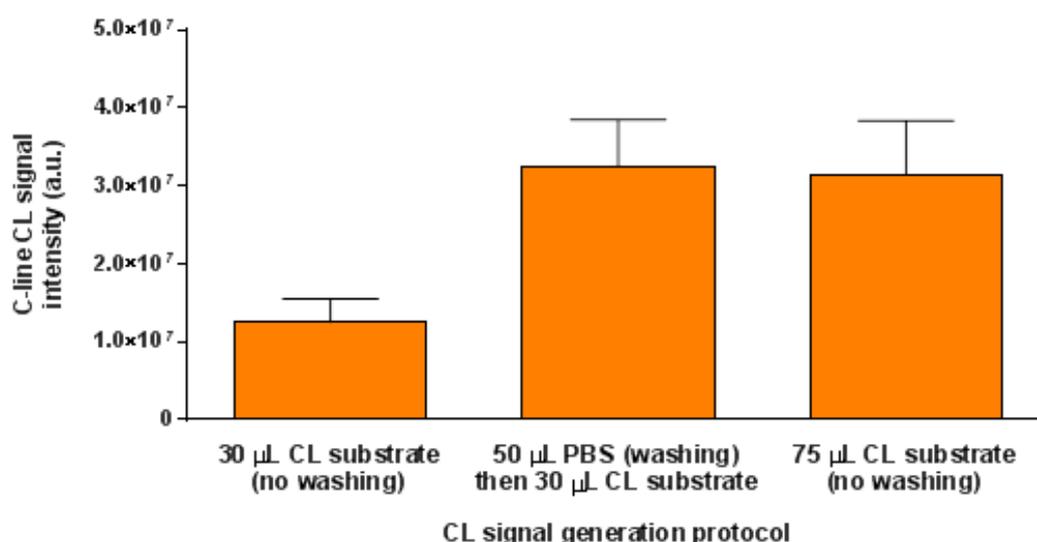


Figure S4: Mean CL signals ($n = 3$) measured in the C-line during analysis of cortisol-free oral fluid samples using different protocols for CL signal generation: (a) loading of 30 μ l of CL substrate on the sample pad (no washing); (b) washing with 50 μ l of PBS followed by loading of 30 μ l of CL substrate on the sample pad; (c) loading of 75 μ l of CL substrate on the sample pad (no washing).

3.1.7 Method performance

Assay accuracy was also evaluated by analysing 10 saliva samples and comparing the results with those obtained using a commercial ELISA kit for salivary cortisol obtained from Diametra. The results shown in Figure S5 showed a good correlation between the two assays, with recovery values comprised between 84% and 112%.

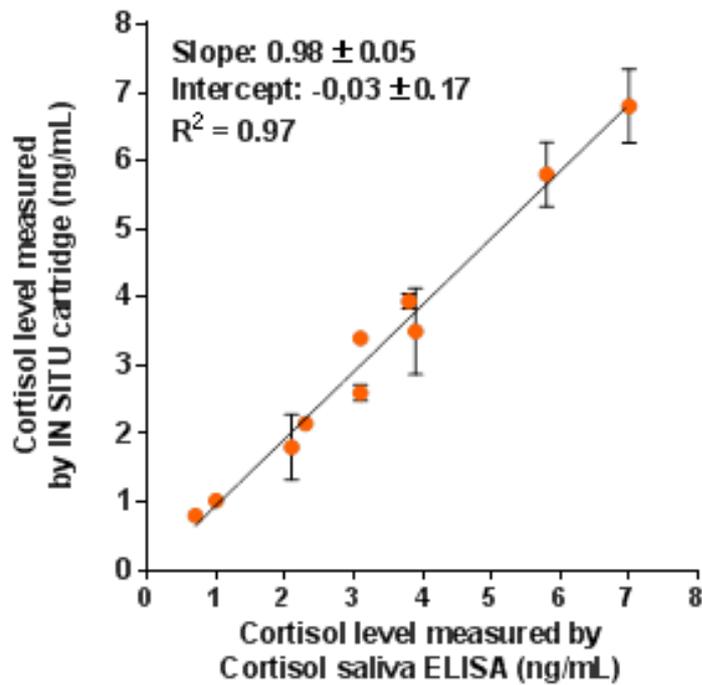


Figure S5: Comparison of the cortisol levels measured in 10 saliva samples using the IN SITU LFIA cartridge and the commercial ELISA kit for salivary cortisol.