

Alma Mater Studiorum Università di Bologna  
Archivio istituzionale della ricerca

Update of the simplified criteria for autoimmune hepatitis: Evaluation of the methodology for immunoserological testing

This is the final peer-reviewed author's accepted manuscript (postprint) of the following publication:

*Published Version:*

Johanna Galaski, Christina Weiler-Normann, Miriam Schakat, Kalliopi Zachou, Paolo Muratori, Sibylle Lampalzer, et al. (2021). Update of the simplified criteria for autoimmune hepatitis: Evaluation of the methodology for immunoserological testing. JOURNAL OF HEPATOLOGY, 74(2), 312-320 [10.1016/j.jhep.2020.07.032].

*Availability:*

This version is available at: <https://hdl.handle.net/11585/807898> since: 2021-02-26

*Published:*

DOI: <http://doi.org/10.1016/j.jhep.2020.07.032>

*Terms of use:*

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>).  
When citing, please refer to the published version.

(Article begins on next page)

This is the final peer-reviewed accepted manuscript of:

Galaski J, Weiler-Normann C, Schakat M, Zachou K, Muratori P, Lampalzer S, et al. Update of the simplified criteria for autoimmune hepatitis: Evaluation of the methodology for immunoserological testing. *Journal of Hepatology* 2021;74:312–20. <https://doi.org/10.1016/j.jhep.2020.07.032>.

The final published version is available online at:

<https://doi.org/10.1016/j.jhep.2020.07.032>

Terms of use:

Some rights reserved. The terms and conditions for the reuse of this version of the manuscript are specified in the publishing policy. For all terms of use and more information see the publisher's website.

*This item was downloaded from IRIS Università di Bologna (<https://cris.unibo.it/>)*

***When citing, please refer to the published version.***

1 **Update of the simplified criteria for autoimmune hepatitis: evaluation of the**  
2 **methodology for immunoserological testing**

3  
4  
5  
6  
7 4 Johanna Galaski<sup>1\*</sup>, Christina Weiler-Normann<sup>1,2,7\*</sup>, Miriam Schakat<sup>1</sup>, Kalliopi  
8  
9 5 Zachou<sup>3</sup>, Paolo Muratori<sup>4,7</sup>, Sibylle Lampalzer<sup>1</sup>, Friedrich Haag<sup>5</sup>, Christoph  
10  
11 6 Schramm<sup>1,2,7</sup>, Marco Lenzi<sup>6,7</sup>, George N. Dalekos<sup>3</sup>, Ansgar W. Lohse<sup>1,7</sup>

12  
13  
14  
15  
16  
17 8 <sup>1</sup>I. Department of Medicine, University Medical Center Hamburg-Eppendorf,  
18  
19 9 Hamburg, Germany; <sup>2</sup>Martin Zeitz Center for Rare Diseases, University Medical  
20  
21 10 Center Hamburg-Eppendorf, Hamburg, Germany; <sup>3</sup>Institute of Internal Medicine and  
22  
23 11 Hepatology, Department of Medicine and Research Laboratory of Internal Medicine,  
24  
25 12 National Expertise Center of Greece in Autoimmune Liver Diseases, General  
26  
27 13 University Hospital of Larissa, Larissa, Greece; <sup>4</sup>Department for Life Quality Studies,  
28  
29 14 Alma Mater Studiorum, University of Bologna, Bologna, Italy; <sup>5</sup>Institute of  
30  
31 15 Immunology, University Medical Center Hamburg-Eppendorf, Hamburg, Germany;  
32  
33 16 <sup>6</sup>Center for the Study and Treatment of Autoimmune Diseases of the Liver and Biliary  
34  
35 17 System, Department of Medical and Surgical Sciences (DIMEC), University of  
36  
37 18 Bologna, Italy; <sup>7</sup>European Reference Network on Hepatological Diseases (ERN  
38  
39 19 RARE-LIVER).

40  
41  
42  
43  
44 20 \*Equally contributing authors

45  
46  
47  
48  
49 21

50  
51 22 **Corresponding author**

52  
53 23 Ansgar W. Lohse

54  
55  
56 24 I. Department of Medicine, University Medical Center Hamburg-Eppendorf,  
57  
58 25 Martinstraße 52, 20246 Hamburg, Germany.

59  
60 26 Tel. +49 (0)40 741053910; Fax. +49 (0)40 741058531

61  
62  
63  
64  
65

27 Email: a.lohse@uke.de

28 Key words: autoantibodies, antinuclear antibodies, smooth muscle antibodies, F-  
29 actin, immunofluorescence, ELISA

30

31 Electronic word count; abstract: 249; manuscript: 3913

32 Number of tables: 4; number of figures: 4

33

### 34 **Conflict of Interest**

35 Weiler-Normann C reports speaker's fees from Euroimmun and Werfen (Inova) to her  
36 institution. All other authors declare no conflict of interest with respect to this study.

37

### 38 **Financial support**

39 Supported by the German Research Foundation (SFB 841 to CS, CWN and AWL  
40 and KFO306 to CS and AWL), the YAEL Foundation, and the Helmut and Hannelore  
41 Greve Foundation (CS).

42

### 43 **Data availability statement**

44 The dataset generated during this study is available from the corresponding author  
45 upon reasonable request.

46

### 47 **Author contributions**

48 Galaski J: substantial contribution to conception and design, data acquisition and  
49 analysis, interpretation of data, drafting of the article

50 Weiler-Normann C: substantial contribution to conception and design, data  
51 acquisition and interpretation of data, critical revision of the article for important  
52 intellectual content

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

53 Schakat M, Zachou K, Muratori P, Lampalzer S, Haag F, Lenzi M, Dalekos GN:  
54 substantial contribution to data acquisition, critical revision

55 Schramm, C: critical revision of the article for important intellectual content

56 Lohse AW: substantial contribution to conception and design, interpretation of data,  
57 critical revision of the article for important intellectual content

58 All authors approved submission.

### 59 **Lay summary**

60 Autoantibodies are a hallmark of autoimmune hepatitis and are traditionally tested for  
61 by immunofluorescence assays on rodent tissue sections. Herein, we demonstrate  
62 that both HEp-2 cells as substrate for ANA IFT and ELISA-based testing are  
63 potentially reliable alternatives for autoantibody assessment in autoimmune hepatitis.  
64 We propose the implementation of these testing methods into the simplified criteria  
65 for the diagnosis of autoimmune hepatitis.

66

### 67 **Highlights**

- 68 • IFT on HEp-2 cells is a valid alternative to the standard ANA assessment on  
69 rodent tissue sections in AIH when cutoffs titers are increased
- 70 • ANA ELISA and F-actin ELISA represent potential alternatives to IFT in the  
71 diagnosis of AIH
- 72 • ANA ELISA kits should include HEp-2 nuclear extracts to account for  
73 unrecognized autoantigens
- 74 • ELISA cutoffs need to be validated locally to be predictive in diagnosing AIH

75

76

77

78

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

## 79 Abstract

1  
2 80  
3  
4  
5 81 **Background & Aims:** The simplified criteria for the diagnosis of autoimmune  
6  
7 82 hepatitis (AIH) include immunofluorescence testing (IFT) of antinuclear and smooth  
8  
9 83 muscle autoantibodies (ANA and SMA) on rodent tissue sections. We aimed to  
10  
11 84 establish scoring criteria for implementation of ANA IFT on HEp-2 cells and ELISA-  
12  
13 85 based testing. **Methods:** ANA and SMA reactivity of 61 AIH sera and 72 non-  
14  
15 86 alcoholic fatty liver disease (NAFLD) controls were separately assessed on tissue  
16  
17 87 sections and human epithelioma (HEp-2) cells to compare the diagnostic value at  
18  
19 88 increasing titers. A total of 113 AIH patients at diagnosis and 202 controls from three  
20  
21 89 European centers were assessed by IFT as well as three different commercially  
22  
23 90 available ANA ELISA and one anti-F-actin ELISA. **Results:** ANA assessment by IFT  
24  
25 91 on liver sections had 83.6% sensitivity and 69.4% specificity for AIH at a titer of 1:40.  
26  
27 92 On HEp-2 cells, sensitivity and specificity were 75.4% and 73.6%, respectively, at an  
28  
29 93 adjusted titer of 1:160. Area under the curve (AUC) values of ANA ELISA ranged  
30  
31 94 from 0.70 – 0.87, with ELISA coated with HEp-2 extracts in addition to selected  
32  
33 95 antigens performing significantly better. SMA assessment by IFT had the highest  
34  
35 96 specificity for the SMA-VG/T pattern and anti-MF reactivity on HEp-2 cells. ELISA-  
36  
37 97 based anti-F-actin evaluation was a strong predictor of AIH (AUC 0.88) and  
38  
39 98 performed better than SMA assessment by IFT (AUC 0.77 – 0.87). **Conclusion:** At  
40  
41 99 adjusted cutoffs, both ANA IFT using HEp-2 cells and ELISA-based autoantibody  
42  
43 100 evaluation for ANA and SMA are potential alternatives to tissue-based IFT for the  
44  
45 101 diagnosis of AIH.  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57

## 58 103 Introduction

59  
60 104  
61  
62  
63  
64  
65

105 Autoimmune hepatitis (AIH) is a chronic immune-mediated liver disease. Due to  
1  
2 106 heterogeneity of the presentation, the diagnosis remains challenging. An early  
3  
4 107 diagnosis is, however, critical for timely initiation of life-saving immunosuppressive  
5  
6  
7 108 therapy. To assist diagnostic evaluation, a simplified diagnostic score was  
8  
9  
10 109 established by the International Autoimmune Hepatitis Group (IAIHG) in 2008 for use  
11  
12 110 in clinical practice [1]. Scoring criteria include characteristic findings on liver  
13  
14 111 histology, the absence of viral hepatitis, an elevation of immunoglobulin G (IgG), and  
15  
16  
17 112 circulating autoantibodies.

18  
19 113 Autoantibodies associated with AIH include antinuclear antibodies (ANA), smooth  
20  
21 114 muscle antibodies (SMA), liver kidney microsomal type 1 (LKM1) antibodies, liver  
22  
23  
24 115 cytosol type 1 (LC1) antibodies, and soluble liver antigen/liver pancreas (SLA/LP)  
25  
26 116 antibodies. Screening for liver disease-associated autoantibodies is traditionally  
27  
28  
29 117 performed by immunofluorescence testing (IFT) on rodent tissue sections.  
30  
31  
32 118 Accordingly, the simplified AIH score refers to autoantibody titers as measured by  
33  
34 119 IFT using tissue sections at a cutoff titer of 1:40. However, in several laboratories,  
35  
36 120 there has been a shift of autoantibody assessment towards human epithelioma (HEp-  
37  
38  
39 121 2) cells rather than tissue sections as substrate for IFT. Furthermore, enzyme-linked  
40  
41 122 immunosorbent assays (ELISA), for which the score does not account for, are  
42  
43  
44 123 frequently used in some countries. In order to make the simplified AIH score usable  
45  
46 124 across the world, adaptation of the score to different immunoserology methods is  
47  
48  
49 125 urgently needed.

50  
51 126 HEp-2 cells are widely used as substrate for ANA evaluation. In addition to a higher  
52  
53 127 sensitivity, characteristic staining patterns evaluated on HEp-2 cells are useful in  
54  
55  
56 128 guiding further confirmatory testing. However, a consensus statement by the IAIHG  
57  
58 129 committee for autoimmune serology advises against the use of HEp-2 cells at a  
59  
60  
61 130 screening stage [2] because of a high positivity rate in healthy individuals at low  
62  
63  
64  
65

131 cutoff titers [3]. If HEp-2 cells are used, the IAHG suggests titers should be halved  
1  
2 132 for the simplified score to be applicable [1]. However, this possible correction factor  
3  
4  
5 133 suggestion has never been validated by comparative studies [4].  
6

7 134 SMA constitute a heterogeneous group of autoantibodies that primarily target F-actin,  
8  
9  
10 135 [5]. On kidney tissue sections, Bottazzo and colleagues distinguished three  
11  
12 136 immunofluorescence patterns: SMA-V (vessels), SMA-VG (vessels/glomeruli), and  
13  
14 137 SMA-VGT (vessels/ glomeruli/ tubuli) [6]. In contrast to the SMA-V pattern, SMA-  
15  
16  
17 138 VG/T correlates with F-actin reactivity and is more specific for AIH [6-8]. Similarly,  
18  
19 139 anti-F-actin antibodies stain microfilaments (MF) on HEp-2 cells [9]. Overall,  
20  
21  
22 140 sensitivity and specificity of SMA positivity strongly depend on fluorescence patterns,  
23  
24 141 which is not taken into consideration by current AIH scoring systems.  
25

26 142 Since IFT is time-consuming, requires experienced technicians and lacks  
27  
28  
29 143 standardization, ELISA have emerged as a widely used alternative for routine  
30  
31  
32 144 autoantibody testing in many laboratories, especially in the United States. These  
33  
34 145 tests were originally developed for use in the evaluation of rheumatic diseases and  
35  
36 146 their diagnostic value in liver disease is unknown. ELISA testing can minimize  
37  
38  
39 147 interobserver variability inherent to IFT. However, it is unclear whether ELISA can  
40  
41 148 replace IFT for the detection of the heterogeneous autoantibodies ANA and SMA  
42  
43  
44 149 with their range of antigenic specificities. To complicate matters even further, up to  
45  
46 150 30% of ANA-positive AIH patients do not react with any known nuclear antigens [10]  
47  
48  
49 151 and might thus be missed by ELISA testing, which are based primarily on known  
50  
51 152 nuclear antigens. In addition, commercially available ANA ELISA lack standardization  
52  
53 153 – they differ in their antigenic profiles and assay-specific cutoff values.  
54

55  
56 154 Taken together, the AIH simplified score does not account for ANA and SMA as  
57  
58 155 evaluated by IFT on HEp-2 cells or for ELISA, even though these tests are widely  
59  
60  
61 156 used. We therefore set out to study the diagnostic validity of IFT and ELISA-based  
62  
63  
64  
65



157 autoantibody testing for the diagnosis of AIH to make these applicable in diagnosing  
1 158 AIH.

2 159

## 3 160 **Patients and methods**

4 161

### 5 162 **Study population**

6 163 This multicenter study included a total of 113 patients with AIH at diagnosis and 202  
7 164 controls (82 NAFLD patients, 99 primary sclerosing cholangitis (PSC) patients and 21  
8 165 healthy controls) from three centers: Hamburg (Germany), Bologna (Italy), and  
9 166 Larissa (Greece). A flow-chart of patient cohorts is shown in Figure 1. The large  
10 167 majority of AIH patients (106/113, 93.8%) were treatment-naïve at the time of  
11 168 sampling. In addition, sera from 26 patients with primary biliary cholangitis (PBC)  
12 169 were tested and analyzed separately. Sera were collected between December 2006  
13 170 and March 2020 and stored at -80°C until use. The study was approved by the local  
14 171 ethics committee (PV4081-0005, PV 4081-0008).

15 172 The diagnosis of AIH was based on clinical, serological, and histopathological  
16 173 criteria, consistent with the EASL clinical practice guidelines [11], and confirmed by  
17 174 long-term follow-up in all patients. Patients with AIH and features of PSC or PBC  
18 175 were excluded from the study. Diagnoses of disease controls were based on  
19 176 established diagnostic criteria [12-14]. Blood donors with liver enzymes within the  
20 177 normal range, negative for HBV/HCV, and negative for autoantibodies by IFT were  
21 178 included as healthy controls.

22 179

### 23 180 **Autoantibody assessment by IFT**

24 181 IFT was performed in the respective center in which sera were collected. At the  
25 182 University Medical Center Hamburg-Eppendorf sera were tested using a Biochip

183 Mosaic of primate liver, rat kidney, and rat stomach tissue sections as well as human  
1  
2 184 epithelioma (HEp-2) cells (Mosaic Basic Profile 3, Euroimmun, Germany). The assay  
3  
4  
5 185 was performed manually according to the manufacturer's instructions at a dilution of  
6  
7 186 1:40. Further dilutions up to 1:1280 were processed by the Helios automated IFA  
8  
9  
10 187 system (Aesku Diagnostics, Wendelsheim, Germany), using the same substrates  
11  
12 188 and conditions. Reactivity patterns were assessed under a fluorescence microscope  
13  
14 189 (Eurostar, Euroimmun, Germany). ANA and SMA reactivity were separately  
15  
16  
17 190 evaluated on all four substrates. SMA reactivity on kidney sections was assessed  
18  
19 191 according to Bottazzo et al. [6]. The observers were blinded to clinical data.

21  
22 192 Sera from the University Hospital of Bologna, Italy, were tested by IFT on both tissue  
23  
24 193 sections and HEp-2 cells (Euroimmun, Germany) and were automatically processed  
25  
26  
27 194 at a starting dilution of 1:80 up to 1:640. ANA titers were mainly reported as  
28  
29 195 assessed on HEp-2 cells and thus these data were used for comparison with ANA  
30  
31 196 ELISA.

33  
34 197 Sera from the University Hospital of Larissa, Greece, were tested by  
35  
36 198 immunofluorescence on in-house fresh cryostat liver, kidney and stomach rat  
37  
38  
39 199 sections and HEp-2 cells (Inova Diagnostics). ANA titers were mainly reported as  
40  
41 200 assessed on tissue sections and thus these data were used for comparison with ANA  
42  
43  
44 201 ELISA. Sera were processed manually at a starting dilution of 1:40 up to 1:640.

45  
46 202

#### 48 203 **Detection of antinuclear and F-actin antibodies by ELISA**

50  
51 204 All ELISA testing was performed at the University Medical Center Hamburg-  
52  
53 205 Eppendorf. Antinuclear antibodies were assessed using enzyme immunoassays from  
54  
55  
56 206 three different manufacturers (Quanta Lite ANA ELISA, Inova Diagnostics, US; ANA  
57  
58 207 Screening Test, Bio-Rad, US; ANA Screen ELISA, Euroimmun, Germany). All assays  
59  
60  
61 208 detect autoantibodies of IgG subtype and display antigenic specificities to dsDNA,

62  
63  
64  
65

209 histones, Sm/RNP, SS-A, SS-B, Scl-70, centromere, and Jo-1. The Quanta Lite ANA  
1  
2 210 ELISA is additionally coated with highly purified proliferating cell nuclear antigen  
3  
4 211 (PCNA), mitochondrial M2 antigen, and ribosomal-P proteins. Besides individual  
5  
6  
7 212 antigens, immunoassays from both Inova Diagnostics and Bio-Rad include HEp-2  
8  
9 213 cell nuclei extracts.

10  
11  
12 214 Antibodies to F-actin were detected using a commercial ELISA (Quanta Lite Actin  
13  
14 215 IgG, Inova Diagnostics, US). All enzyme immunoassays were performed in  
15  
16  
17 216 duplicates according to the manufacturer's recommendations. Investigators who  
18  
19 217 carried out immunoassays were blinded to clinical data and the results of IFT.

20  
21  
22 218

### 23 24 219 **Statistical analyses**

25  
26 220 Data was expressed as median (range), or n (%) as appropriate. Statistical  
27  
28  
29 221 significance between groups was assessed with Fisher's exact test for categorical  
30  
31 222 variables and the Mann-Whitney *U* test for continuous variables. Correlations were  
32  
33  
34 223 evaluated using Spearman correlation coefficients. The diagnostic value of variables  
35  
36 224 in discriminating AIH from controls was assessed by receiver operating characteristic  
37  
38  
39 225 (ROC) analysis. Statistical significance between area under the curve (AUC) values  
40  
41 226 was assessed by the DeLong test. All reported *P* values are based on two-sided  
42  
43  
44 227 tests and a *P* value < 0.05 was considered statistically significant. Statistical analyses  
45  
46 228 were performed using GraphPad Prism (version 6), IBM SPSS (version 23), and R  
47  
48 229 software (version 3.5.1).

49  
50  
51 230

### 52 53 231 **Results**

54  
55  
56 232

### 57 58 233 **Comparison of HEp-2 cells and tissue sections as substrates for ANA IFT**

59  
60  
61  
62  
63  
64  
65

234 We first investigated the diagnostic value of HEp-2 cells in comparison to tissue  
1  
2 235 sections as substrates for ANA IFT in the context of AIH. To this end, sera from 61  
3  
4 236 AIH patients and 72 patients with biopsy-proven NAFLD treated at the University  
5  
6  
7 237 Medical Center Hamburg-Eppendorf were evaluated for autoantibodies by IFT.  
8  
9  
10 238 Clinical characteristics of the patient groups at the time of sampling are summarized  
11  
12 239 in supplemental Table 1.  
13  
14 240 Sensitivity and specificity of ANA IFT for HEp-2 cells and tissue sections are shown  
15  
16  
17 241 in Table 1. Among tissue sections, primate liver showed the highest diagnostic value  
18  
19 242 for ANA evaluation. Sensitivity and specificity were 83.6% and 69.4% at a titer of  
20  
21  
22 243 1:40, respectively, and 68.9% and 80.6% at a titer of 1:80, respectively. Specificity  
23  
24 244 increased to 91.7% at a titer of 1:160 at the cost of a lower sensitivity of 47.5%. As  
25  
26 245 expected, the use of HEp-2 cells led to higher titers. Specificity was inadequate at a  
27  
28  
29 246 1:40 dilution. At a titer of 1:80, sensitivity was 91.8% at a low specificity of 36.1%. At  
30  
31  
32 247 higher titers, sensitivity and specificity were comparable to those observed on liver  
33  
34 248 sections: 75.4% and 73.6%, respectively, at a titer of 1:160; 72.1% and 76.4%,  
35  
36 249 respectively, at a titer of 1:320. The homogenous pattern was significantly more  
37  
38  
39 250 frequent in AIH patients (41.0%) than in NAFLD patients (6.9%,  $P < 0.001$ ).

41 251  
42  
43  
44 252 **Sensitivity and specificity of SMA fluorescence patterns on tissue sections and**  
45  
46 253 **HEp-2 cells**

47  
48 254 We next assessed the diagnostic value of several SMA fluorescence patterns at  
49  
50  
51 255 different titers (Table 2). As expected, at a 1:40 titer, the SMA-V pattern on kidney  
52  
53 256 sections, staining of smooth muscle on stomach sections as well as consideration of  
54  
55  
56 257 any SMA positivity resulted in a low specificity of 33.3% – 45.8%. In contrast, the  
57  
58 258 SMA-VG pattern was more specific for the diagnosis of AIH even at low titers.  
59  
60  
61 259 Sensitivity and specificity were 72.1% and 70.8%, respectively, at a titer of 1:40, and  
62  
63  
64  
65

260 65.6% and 88.9%, respectively, at a titer of 1:80. The highest specificity was seen for  
261 the SMA-VGT pattern and anti-MF reactivity on HEp-2 cells. At a 1:40 dilution,  
262 specificity was 93.1% – 94.4% at a sensitivity of 52.5% – 60.7%. Of note, with  
263 increasing titers, staining of the SMA-VGT pattern first faded for tubuli, then  
264 glomeruli, and finally vessels. In other terms, the SMA-VGT pattern changed to SMA-  
265 VG and finally to SMA-V with increasing dilutions. Taken together, SMA positivity  
266 was highly specific even at low titers for SMA-VG/T and anti-MF reactivity on HEp-2  
267 cells, but only at higher titers for other SMA patterns.

### 269 **ELISA-based autoantibody testing for the diagnosis of AIH**

270 We next assessed the diagnostic value of ELISA-based autoantibody evaluation to  
271 discriminate between AIH and controls. Sera from three European centers were  
272 reassessed by three different ANA ELISA and one F-actin ELISA. Clinical  
273 characteristics of the patient groups at the time of sampling are summarized in  
274 supplemental Tables 1 – 3.

275 ANA testing by the Bio-Rad and Inova ANA ELISA had a similar diagnostic accuracy  
276 (AUC 0.85 and 0.87, respectively;  $P = 0.32$ ) and performed significantly better  
277 compared to the ANA Euroimmun ELISA (AUC 0.70;  $P < 0.001$ ) (Figure 2A).

278 Correlation analyses between the ANA ELISA results found the strongest correlation  
279 between the Bio-Rad and Inova ANA ELISA ( $r_s = 0.72$ ;  $P < 0.001$ ) (Supplemental  
280 Figure 1). Test characteristics of the ANA ELISA kits varied greatly at cutoffs  
281 recommended by the manufacturers. In fact, sensitivity and specificity were 65.5%  
282 and 88.6% for the Bio-Rad assay (recommended cutoff  $\geq 1$  RU), 79.6% and 78.2%  
283 for the ANA Inova assay (recommended cutoff  $\geq 20$  RU), and 22.1% and 95.0% for  
284 the ANA Euroimmun assay (recommended cutoff  $\geq 1$  RU), respectively (Table 3).

285 Like for ANA, we assessed the diagnostic value of a F-actin ELISA. ROC analysis  
1  
2 286 revealed anti-F-actin as a strong predictor of AIH (AUC 0.89) (Figure 2B). At a cutoff  
3  
4 287 of 20 RU, sensitivity and specificity were 81.4% and 82.2%, respectively; at a cutoff  
5  
6  
7 288 of 30 RU, sensitivity and specificity were 66.4% and 92.6%, respectively (Table 3).  
8  
9 289 Importantly, anti-F-actin was still a predictor of AIH in the subgroup of patients with  
10  
11  
12 290 normal range IgG ( $\leq 16$  g/l;  $n = 35/109$ ) (AUC 0.79).  
13

### 14 291 **ELISA- compared to IFT-based evaluation of autoantibodies**

15  
16  
17 292 We next compared ELISA- and IFT-based ANA evaluation. To account for the inter-  
18  
19 293 laboratory variability inherent to IFT, ELISA assessment was compared to IFT results  
20  
21  
22 294 obtained by the respective centers according to local standards. Figure 3 and 4 show  
23  
24 295 the diagnostic performance of ELISA vs. IFT for ANA and SMA/F-actin, respectively,  
25  
26 296 for each center. ANA testing by ELISA and IFT performed similarly for all cohorts,  
27  
28  
29 297 except for the Euroimmun ELISA that showed a significantly lower AUC compared to  
30  
31  
32 298 IFT for the Hamburg cohort (Euroimmun ANA ELISA, AUC 0.65; ANA IFT, AUC 0.82  
33  
34 299 – 0.83;  $P < 0.001$ ).  
35  
36 300

37  
38  
39 301 In addition to the patient groups shown in Figure 1, we tested sera from 26 PBC  
40  
41 302 patients known to frequently present with ANA. Clinical characteristics of PBC  
42  
43  
44 303 patients are detailed in supplemental Table 4. While 17/26 (65.4%) of PBC patients  
45  
46 304 tested positive for ANA by IFT on HEp-2 cells at a cut-off of 1:80, 23/26 (88.4%) and  
47  
48  
49 305 25/26 (96.2%) tested positive by the Bio-Rad and Inova ANA ELISA, respectively.  
50  
51 306 Importantly, median values of the Inova ANA ELISA were significantly higher in PBC  
52  
53 307 patients compared to AIH patients (49.6 RU AIH vs. 161.7 RU PBC;  $P < 0.001$ ) while  
54  
55  
56 308 there was no statistical significant difference for the Bio-Rad ELISA (1.6 RU AIH vs.  
57  
58 309 2.0 RU PBC;  $P = 0.25$ ).  
59  
60  
61  
62  
63  
64  
65

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

310 The F-actin ELISA yielded higher AUC values compared to IFT for each center,  
311 reaching statistical significance for the Hamburg cohort when compared to anti-MF  
312 reactivity on HEp-2 cells (F-actin ELISA, AUC 0.86; anti-MF AUC 0.79;  $P = 0.003$ )  
313 and for the Bologna cohort when compared to any SMA reactivity (F-actin ELISA,  
314 AUC 0.93; any SMA, AUC 0.77;  $P = 0.002$ ).

315 We further assessed the performance of ELISA-based autoantibody testing in the  
316 subgroup of patients with a histological diagnosis of liver cirrhosis. Overall, 24 AIH  
317 patients and 15 controls (4 PSC patients, 11 NAFLD patients) with cirrhosis were  
318 identified. ANA IFT assessed on tissue sections (available for  $n = 35$ ; 20 AIH patients  
319 vs. 15 controls) reached an AUC of 0.84 whereas ELISA-based ANA assessment  
320 yielded higher AUC values of 0.88 – 0.93, without reaching statistical significance  
321 (supplemental Figure 2A). In contrast, anti-F-actin ( $n = 39$ ) was again a strong  
322 predictor of AIH (AUC 0.91) and performed significantly better than SMA assessment  
323 by IFT (SMA-VG/T; AUC 0.80;  $P = 0.049$ ) (supplemental Figure 2B).

### 324 325 **Concordance between IFT- and ELISA-based ANA testing**

326 We next assessed concordance between IFT- and ELISA-based autoantibody testing  
327 and were specifically interested in the proportion of AIH patients that tested positive  
328 by IFT but were missed when tested by ELISA. Of 51 AIH patients from the Hamburg  
329 cohort that tested positive for ANA by IFT on liver tissue sections, the ANA ELISA by  
330 Inova, Bio-Rad and Euroimmun detected 40/51 (78.4%), 28/51 (54.9%), and 10/51  
331 (19.6%) cases at recommended cut-offs, respectively. Conversely, of 10 AIH patients  
332 that tested negative for ANA by IFT, 6 (60%) tested positive by the Inova ELISA and  
333 4 (40%) by the Bio-Rad ELISA. Furthermore, the Inova and Bio-Rad assays detected  
334 all but one of ANA-positive AIH cases from the Larissa and Bologna cohorts.

335 Together, the ROC analysis indicates that ELISA represent a potential alternative to  
1  
2 336 IFT-based autoantibody assessment. However, assays vary considerably in their  
3  
4  
5 337 performance and cut-offs need to be validated for the diagnosis of AIH. If these  
6  
7 338 aspects are taken under consideration and local cut-offs established, ELISA-based  
8  
9  
10 339 autoantibody testing as proposed in Table 4 can be used in the diagnostic work-up of  
11  
12 340 liver disease patients.

## 14 341 15 16 17 342 **Discussion**

18  
19 343  
20  
21  
22 344 This is the first study to comprehensively evaluate IFT- and ELISA-based  
23  
24 345 assessment of ANA and SMA/anti-F-actin in AIH. In analogy to the simplified IAIHG  
25  
26 346 diagnostic score that largely refers to autoantibody assessment as evaluated by IFT  
27  
28  
29 347 on tissue sections, we propose the implementation of autoantibody testing as  
30  
31 348 measured by IFT on HEp-2 cells and ELISA.

32  
33  
34 349 We first aimed to validate the use of HEp-2 cells as substrate for ANA IFT in patients  
35  
36 350 with AIH. As expected, at low titers, ANA as evaluated on HEp-2 cells showed a high  
37  
38  
39 351 sensitivity at the expense of a low specificity. It is precisely the low specificity at a  
40  
41 352 1:40 titer that led the IAIHG to advise against use of HEp-2 cells for ANA evaluation  
42  
43  
44 353 at a screening stage [2]. However, to our knowledge, the diagnostic value of ANA IFT  
45  
46 354 on HEp-2 cells has not been assessed at higher titers in the context of liver disease.

47  
48 355 A previous study investigating ANA IFT in liver disease reported an increased  
49  
50  
51 356 sensitivity of ANA IFT using HEp-2 cells, but was restricted to a 1:40 dilution [15].  
52  
53 357 Our results suggest that HEp-2 cells are a valid alternative to tissue sections, if  
54  
55  
56 358 threshold titers are adapted. We here propose increasing cutoff titers to 1:160 and  
57  
58 359 1:320 for the simplified diagnostic score to be applicable. As outlined above, a cutoff  
59  
60  
61 360 titer of 1:160 is also the recommended cutoff for ANA screening in rheumatic  
62  
63  
64  
65



361 diseases [16]. However, titers vary depending on reagents and equipment used and  
1  
2 362 should be validated locally. In addition, the difference in immunofluorescence  
3  
4  
5 363 intensity between tissue sections and HEp-2 cells is not the same for all subtypes of  
6  
7 364 ANA, but highly dependent on the respective ANA pattern. Nevertheless, overall,  
8  
9  
10 365 HEp-2 cells are a valid alternative to tissue sections for ANA evaluation in AIH.

11  
12 366 We further compared the diagnostic value of different SMA patterns for the diagnosis  
13  
14 367 of AIH. In line with a study by Muratori and colleagues [9], we found that specificity  
15  
16  
17 368 was highest for SMA-VGT and anti-MF reactivity at a titer of 1:40. Complementing  
18  
19 369 this previous study, we additionally assessed SMA patterns at further dilutions.  
20  
21  
22 370 Interestingly, sensitivity and specificity of generic SMA at higher titers was  
23  
24 371 comparable to the diagnostic value of SMA-VG/T and anti-MF reactivity at a 1:40  
25  
26  
27 372 titer. Furthermore, as previously described [6], we observed a shift from SMA-VGT  
28  
29 373 to SMA-G and then SMA-V with increasing dilutions for individual samples. It thus  
30  
31  
32 374 appears likely that the SMA-VGT pattern is a reflection of high-titer SMA with  
33  
34 375 specificity for F-actin. In contrast, the SMA-V pattern can be seen for both low-titer  
35  
36 376 SMA with anti-F-actin reactivity or SMA targeting other cytoskeletal components.  
37  
38  
39 377 Taken together, our results add to the literature [6, 7, 9] that highlights the  
40  
41 378 importance of reporting SMA patterns, in both the scientific and clinical context.

42  
43  
44 379 Several studies have assessed ANA evaluation by ELISA in rheumatic diseases [17-  
45  
46 380 21], but analogous studies in AIH are lacking. To fill this gap, we assessed the  
47  
48  
49 381 diagnostic value of three different ANA ELISA in AIH patients. We observed  
50  
51 382 significant differences depending on the ELISA used, with the Bio-Rad and Inova  
52  
53 383 assays performing best. In contrast, at the cut-off recommended by the  
54  
55  
56 384 manufacturer, the Euroimmun ANA ELISA had a low sensitivity of 22.1% at a 95%  
57  
58 385 specificity. These results might be explained by differing ELISA formulations. Indeed,  
59  
60  
61 386 both the Inova and Bio-Rad ANA ELISA include HEp-2 nuclear extracts in addition to  
62  
63  
64  
65

387 recombinant and purified nuclear antigens to account for unrecognized autoantigens.

1  
2 388 In contrast, the Euroimmun assay is only comprised of selected nuclear antigens. Its  
3  
4  
5 389 antigenic specificities are therefore better defined, ensuring high specificity for the  
6  
7 390 diagnosis of rheumatic diseases. However, our data suggest that this comes at the  
8  
9  
10 391 cost of a low diagnostic value in autoimmune hepatitis. With regard to ELISA  
11  
12 392 formulations, it is also worth mentioning that the Inova ANA ELISA is the only assay  
13  
14 393 in this study including purified ribosomal P and mitochondrial M2 antigen. In a study  
15  
16  
17 394 by Calich and colleagues, autoantibodies against ribosomal P were found in 9/93  
18  
19 395 (9.7%) AIH patients and none of the healthy controls [22]. In contrast, the  
20  
21  
22 396 incorporation of mitochondrial antigens is not expected for an ANA screening assay  
23  
24 397 and carries considerable potential for confusion. Indeed, if the Inova ANA ELISA  
25  
26  
27 398 were to be used for the diagnostic workup of elevated liver enzymes, distinction  
28  
29 399 between ANA and antimitochondrial antibodies (AMA) would not be possible in a  
30  
31  
32 400 reasonable fashion. Incorporation of mitochondrial antigens also likely explains the  
33  
34 401 significantly higher values of the Inova ANA ELISA in PBC patients compared to AIH  
35  
36 402 patients. Overall, while the careful choice of ELISA formulation and validation of cut-  
37  
38  
39 403 offs is critical, our data suggest that in principle ELISA testing represents a potentially  
40  
41 404 good alternative to ANA IFT. Importantly, if ELISA-based autoantibody assessment is  
42  
43  
44 405 negative despite clinical suspicion of AIH, additional IFT should be performed.

45  
46 406 In the present study, we further compared IFT-based SMA evaluation to an anti-F-  
47  
48  
49 407 actin ELISA. Consistent with previous results [23], we found that anti-F-actin had a  
50  
51 408 significantly higher diagnostic value for the diagnosis of AIH. Interestingly, while  
52  
53 409 hypergammaglobulinemia potentiated the predictive value of anti-F-actin for the  
54  
55  
56 410 diagnosis of AIH, F-actin autoantibodies were still a strong predictor of AIH in the  
57  
58 411 subgroup of AIH patients with IgG within the normal range (AUC 0.79).

59  
60  
61  
62  
63  
64  
65

412 Several limitations to the present study warrant further discussion. First, IFT allows  
1  
2 413 for the detection of additional autoantibodies such as AMA and provides  
3  
4 414 characteristic staining patterns that point towards antigenic specificities of ANA. The  
5  
6  
7 415 benefit of this relevant information was not assessed in the present study. While ANA  
8  
9  
10 416 ELISA do not provide such additional information, some specific and reliable tests  
11  
12 417 exist to further assess antigen specificity of ANA-positive sera. Indeed, most of the  
13  
14 418 PBC sera we tested were highly positive both in the Inova ANA ELISA, which does  
15  
16  
17 419 however also include M2 antigen, the key target of antimitochondrial antibodies  
18  
19 420 characteristic of PBC, as well as in the Bio-Rad ANA ELISA. Thus, for discrimination  
20  
21  
22 421 between AIH and PBC sera, further systematic testing by a specific M2-AMA ELISA  
23  
24 422 and by sp100 and gp210 ELISA would be required. However, this would have been  
25  
26 423 beyond the scope of the present study.

27  
28  
29 424 Second, we included only one F-actin ELISA. However, compared to the  
30  
31 425 heterogeneous group of ANA, F-actin is a defined antigen and the F-actin ELISA  
32  
33  
34 426 used in this study was investigated in two previous studies [7, 23].

35  
36 427 Furthermore, while control cohorts were well characterized, relevant patient groups  
37  
38  
39 428 such as drug-induced liver injury patients were not included in the present study.

40  
41 429 Finally, the gender distribution between AIH and controls was somewhat unbalanced  
42  
43  
44 430 reflecting the natural sex differences in these conditions. Although this potentially  
45  
46 431 influenced the frequency of autoantibodies in patient groups, it most probably did not  
47  
48  
49 432 affect how the various autoantibody assays compared to one another.

50  
51 433 In conclusion, our results suggest that both IFT evaluation on HEp-2 cells as well as  
52  
53 434 ELISA-based autoantibody assessment are potential alternatives to IFT on tissue  
54  
55  
56 435 sections. Our data indicate that (1) HEp-2 cells can be used for ANA assessment in  
57  
58 436 AIH if scoring cutoff titers are increased, (2) The SMA-VG/T pattern and anti-MF  
59  
60  
61 437 reactivity on HEP-2 cells are highly specific even at low titers while generic SMA is  
62  
63  
64  
65

438 specific only at higher titers, (3) ANA and F-actin ELISA show at least equivalent  
1  
2 439 diagnostic performance compared to IFT, but ELISA kits for ANA assessment should  
3  
4 440 include HEp-2 nuclear extracts to account for unknown nuclear antigens and cutoffs  
5  
6  
7 441 need to be validated for the use in AIH. In the future, cut-off values for autoantibody  
8  
9 442 testing should be determined and validated by industry on standardized AIH sera and  
10  
11  
12 443 controls and re-validated by diagnostic laboratories, as technical details may  
13  
14 444 influence the exact values. Nonetheless, the objective nature of these tests will make  
15  
16  
17 445 them more attractive in the future avoiding observation errors due to the subjective  
18  
19 446 assessment of staining patterns as in SMA testing on tissue sections. Based on our  
20  
21  
22 447 results, under the prerequisite of careful choice of ELISA formulation and validation  
23  
24 448 of cut-offs, we propose an adaptation of the simplified diagnostic score for AIH as  
25  
26  
27 449 summarized in Table 4 for everyday use in different laboratory settings.  
28

29 450

30  
31 451

32  
33  
34 452

35  
36 453

37  
38  
39 454

40  
41 455

42  
43  
44 456

45  
46 457

47  
48  
49 458

50  
51 459

52  
53 460

54  
55  
56 461

57  
58 462

59  
60  
61 463

62

63  
64  
65

464 **References**

- 1  
2 465 [1] Hennes EM, Zeniya M, Czaja AJ, Pares A, Dalekos GN, Krawitt EL, et al. Simplified criteria for  
3  
4 466 the diagnosis of autoimmune hepatitis. *Hepatology* 2008;48:169-176.  
5  
6 467 [2] Vergani D, Alvarez F, Bianchi FB, Cancado EL, Mackay IR, Manns MP, et al. Liver  
7  
8 468 autoimmune serology: a consensus statement from the committee for autoimmune serology of the  
9  
10 469 International Autoimmune Hepatitis Group. *J Hepatol* 2004;41:677-683.  
11  
12 470 [3] Tan EM, Feltkamp TE, Smolen JS, Butcher B, Dawkins R, Fritzler MJ, et al. Range of  
13  
14 471 antinuclear antibodies in "healthy" individuals. *Arthritis Rheum* 1997;40:1601-1611.  
15  
16 472 [4] Tozzoli R, Villalta D, Bizzaro N. Challenges in the Standardization of Autoantibody Testing: a  
17  
18 473 Comprehensive Review. *Clin Rev Allergy Immunol* 2017;53:68-77.  
19  
20 474 [5] Dighiero G, Lymberi P, Monot C, Abuaf N. Sera with high levels of anti-smooth muscle and  
21  
22 475 anti-mitochondrial antibodies frequently bind to cytoskeleton proteins. *Clin Exp Immunol* 1990;82:52-  
23  
24 476 56.  
25  
26 477 [6] Bottazzo GF, Florin-Christensen A, Fairfax A, Swana G, Doniach D, Groeschel-Stewart U.  
27  
28 478 Classification of smooth muscle autoantibodies detected by immunofluorescence. *J Clin Pathol*  
29  
30 479 1976;29:403-410.  
31  
32 480 [7] Granito A, Muratori L, Muratori P, Pappas G, Guidi M, Cassani F, et al. Antibodies to  
33  
34 481 filamentous actin (F-actin) in type 1 autoimmune hepatitis. *J Clin Pathol* 2006;59:280-284.  
35  
36 482 [8] Liaskos C, Bogdanos DP, Davies ET, Dalekos GN. Diagnostic relevance of anti-filamentous  
37  
38 483 actin antibodies in autoimmune hepatitis. *J Clin Pathol* 2007;60:107-108.  
39  
40 484 [9] Muratori P, Muratori L, Agostinelli D, Pappas G, Veronesi L, Granito A, et al. Smooth muscle  
41  
42 485 antibodies and type 1 autoimmune hepatitis. *Autoimmunity* 2002;35:497-500.  
43  
44 486 [10] Czaja AJ, Nishioka M, Morshed SA, Hachiya T. Patterns of nuclear immunofluorescence and  
45  
46 487 reactivities to recombinant nuclear antigens in autoimmune hepatitis. *Gastroenterology* 1994;107:200-  
47  
48 488 207.  
49  
50 489 [11] EASL Clinical Practice Guidelines: Autoimmune hepatitis. *J Hepatol* 2015;63:971-1004.  
51  
52 490 [12] EASL Clinical Practice Guidelines: management of cholestatic liver diseases. *J Hepatol*  
53  
54 491 2009;51:237-267.  
55  
56 492 [13] European Association for the Study of the Liver. Electronic address eee, European  
57  
58 493 Association for the Study of the L. EASL Clinical Practice Guidelines: The diagnosis and management  
59  
60 494 of patients with primary biliary cholangitis. *J Hepatol* 2017;67:145-172.  
61  
62  
63  
64  
65

- 495 [14] EASL-EASD-EASO Clinical Practice Guidelines for the management of non-alcoholic fatty  
1  
2 496 liver disease. *J Hepatol* 2016;64:1388-1402.
- 3  
4 497 [15] Cassani F, Bianchi FB, Lenzi M, Volta U, Pisi E. Immunomorphological characterisation of  
5  
6 498 antinuclear antibodies in chronic liver disease. *J Clin Pathol* 1985;38:801-805.
- 7  
8 499 [16] Agmon-Levin N, Damoiseaux J, Kallenberg C, Sack U, Witte T, Herold M, et al. International  
9  
10 500 recommendations for the assessment of autoantibodies to cellular antigens referred to as anti-nuclear  
11  
12 501 antibodies. *Ann Rheum Dis* 2014;73:17-23.
- 13  
14 502 [17] Copple SS, Sawitzke AD, Wilson AM, Tebo AE, Hill HR. Enzyme-linked immunosorbent assay  
15  
16 503 screening then indirect immunofluorescence confirmation of antinuclear antibodies: a statistical  
17  
18 504 analysis. *Am J Clin Pathol* 2011;135:678-684.
- 19  
20 505 [18] Reisner BS, DiBlasi J, Goel N. Comparison of an enzyme immunoassay to an indirect  
21  
22 506 fluorescent immunoassay for the detection of antinuclear antibodies. *Am J Clin Pathol* 1999;111:503-  
23  
24 507 506.
- 25  
26 508 [19] Bernardini S, Infantino M, Bellincampi L, Nuccetelli M, Afeltra A, Lori R, et al. Screening of  
27  
28 509 antinuclear antibodies: comparison between enzyme immunoassay based on nuclear homogenates,  
29  
30 510 purified or recombinant antigens and immunofluorescence assay. *Clin Chem Lab Med* 2004;42:1155-  
31  
32 511 1160.
- 33  
34 512 [20] Gniewek RA, Sandbulte C, Fox PC. Comparison of antinuclear antibody testing methods by  
35  
36 513 ROC analysis with reference to disease diagnosis. *Clin Chem* 1997;43:1987-1989.
- 37  
38 514 [21] Fenger M, Wiik A, Hoier-Madsen M, Lykkegaard JJ, Rozenfeld T, Hansen MS, et al. Detection  
39  
40 515 of antinuclear antibodies by solid-phase immunoassays and immunofluorescence analysis. *Clin Chem*  
41  
42 516 2004;50:2141-2147.
- 43  
44 517 [22] Calich AL, Viana VS, Cancado E, Tustumi F, Terrabuio DR, Leon EP, et al. Anti-ribosomal P  
45  
46 518 protein: a novel antibody in autoimmune hepatitis. *Liver Int* 2013;33:909-913.
- 47  
48 519 [23] Frenzel C, Herkel J, Luth S, Galle PR, Schramm C, Lohse AW. Evaluation of F-actin ELISA  
49  
50 520 for the diagnosis of autoimmune hepatitis. *Am J Gastroenterol* 2006;101:2731-2736.  
51  
52 521  
53  
54 522  
55  
56 523  
57  
58 524  
59  
60  
61  
62  
63  
64  
65

525 **Tables**526 **Table 1. Sensitivity and specificity of ANA IFT for different tissue sections**

Substrate	Titer	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
HEp-2 cells	1:40	95.1	8.3	46.8	66.7	48.1
	1:80	91.8	36.1	54.9	83.9	61.7
	1:160	75.4	73.6	70.8	77.9	74.4
	1:320	72.1	76.4	72.1	76.4	74.4
	1:640	60.7	87.5	80.4	72.4	75.2
Primate liver	1:40	83.6	69.4	69.9	83.3	75.9
	1:80	68.9	80.6	75.0	75.3	75.2
	1:160	47.5	91.7	82.9	67.4	71.4
	1:320	47.5	91.7	82.9	67.4	71.4
	1:640	29.5	94.4	81.8	61.3	64.7
Rat kidney	1:40	75.4	73.6	70.8	77.9	74.4
	1:80	65.6	81.9	75.5	73.8	74.4
	1:160	52.5	87.5	78.1	68.5	71.4
	1:320	47.5	91.7	82.9	67.4	71.4
	1:640	34.4	93.1	80.8	62.6	66.2
Rat stomach	1:40	78.7	70.8	69.6	79.7	74.4
	1:80	67.2	81.9	75.9	74.7	75.2
	1:160	52.5	88.9	80.0	68.8	72.2
	1:320	44.3	91.7	81.8	66.0	69.9
	1:640	36.1	93.1	81.5	63.2	66.9
Any tissue positivity (primate liver, rat kidney, rat stomach)	1:40	85.3	65.3	67.5	83.9	74.4
	1:80	73.8	77.8	73.8	77.8	75.9
	1:160	52.5	87.5	78.1	68.5	71.4
	1:320	50.8	91.7	83.8	68.8	72.9
	1:640	37.7	93.1	82.1	63.8	67.7

AIH n=61; NAFLD n=72; ANA, antinuclear antibodies; HEp-2 cells, human epithelioma-2 cells; IFT, immunofluorescence test; NPV, negative predictive value; PPV, positive predictive value.

## 527

528 **Table 2. Sensitivity and specificity of SMA IFT for different patterns**

Substrate	Titer	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
HEp-2 (microfilaments)	1:40	60.7	94.4	90.2	73.9	79.9
	1:80	59.0	98.6	97.3	74.0	80.5
	1:160	54.1	98.6	97.1	71.7	78.2
	1:320	52.5	98.6	97.0	71.0	77.4
	1:640	41.0	100	100	66.7	72.9
Kidney SMA-V (vessels)	1:40	78.7	45.8	55.2	71.7	60.9
	1:80	73.8	72.2	69.2	76.5	72.9
	1:160	68.9	80.6	75.0	75.3	75.2
	1:320	62.3	88.9	82.6	73.6	76.7
	1:640	49.2	98.6	96.8	69.6	75.9
Kidney SMA-VG (vessels, glomeruli)	1:40	72.1	70.8	67.7	75.0	71.4
	1:80	65.6	88.9	83.3	75.3	78.2
	1:160	63.9	94.4	90.7	75.6	80.5
	1:320	55.7	97.2	94.4	72.2	78.2
	1:640	36.1	100	100	64.9	70.7
Kidney SMA-VGT (vessels, glomeruli tubuli)	1:40	52.5	93.1	86.5	69.8	74.4
	1:80	49.2	93.1	85.7	68.4	72.9
	1:160	44.3	95.8	90.0	67.0	72.2
	1:320	31.2	97.2	90.5	62.5	66.9
	1:640	23.0	100	100	60.5	64.7

Kidney SMA-VG or	1:40	75.4	69.4	67.7	76.9	72.2
HEp2	1:80	68.9	88.9	84.0	77.1	79.7
microfilaments	1:160	65.6	94.4	90.9	76.4	81.2
	1:320	62.3	97.2	95.0	75.3	81.2
	1:640	44.3	100	100	67.9	74.4
Liver	1:40	59.0	83.3	75.0	70.6	72.2
(bile canaliculi)	1:80	49.2	95.8	90.9	69.0	74.4
	1:160	42.6	98.6	96.3	67.0	72.9
	1:320	39.3	98.6	96.0	65.7	71.4
	1:640	26.2	100	100	61.5	66.2
Stomach	1:40	83.6	45.8	56.7	76.7	63.2
(tunica muscularis,	1:80	75.4	72.2	69.7	77.6	73.7
lamina muscularis	1:160	72.1	80.6	75.9	77.3	76.7
mucosa, interglandular	1:320	68.9	90.3	85.7	77.4	80.5
fibrils)	1:640	54.1	97.2	94.3	71.4	77.4
Any SMA positivity	1:40	86.9	37.5	54.1	77.1	60.2
	1:80	80.3	69.4	69.0	80.7	74.4
	1:160	72.1	79.2	74.6	77.0	75.9
	1:320	72.1	88.9	84.6	79.0	81.2
	1:640	60.7	97.2	94.9	74.5	80.5

AIH n=61; NAFLD n=72; HEp-2 cells, human epithelioma-2 cells; IFT, immunofluorescence test; NPV, negative predictive value; PPV, positive predictive value; SMA, smooth muscle antibodies; VGT, vessel, glomeruli, tubuli.

**Table 3. Diagnostic value of ANA and F-Actin ELISA at cut-offs recommended by manufacturers**

ELISA	Assay	Cutoff	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
ANA ELISA	Bio-Rad	≥ 1.0	65.5	88.6	76.3	82.1	80.3
		≥ 20	79.6	78.2	67.2	87.3	78.7
	Euroimmun	≥ 30	69.0	86.6	74.3	83.3	80.3
		≥ 1.0	22.1	95.0	71.4	68.6	68.9
F-Actin ELISA	Inova	≥ 20	81.4	82.2	71.9	88.8	81.9
		≥ 30	66.4	92.6	83.3	83.1	83.2

AIH n=113; controls n=202; distribution of diagnoses as shown in Figure 1; ANA, antinuclear antibodies; NPV, negative predictive value; PPV, positive predictive value.

24 529  
 25 530  
 26 531  
 27 532  
 28 532  
 29  
 30  
 31  
 32  
 33  
 34  
 35  
 36  
 37  
 38  
 39 533  
 40 534  
 41 534  
 42 535  
 43 536  
 44 537  
 45 537  
 46 538  
 47 539  
 48 540  
 49 541  
 50 541  
 51 542  
 52 543  
 53 544  
 54 545  
 55 546  
 56 546  
 57 547  
 58 548  
 59 549  
 60 550  
 61 550  
 62  
 63  
 64  
 65



551

**Table 4. Simplified criteria for autoimmune hepatitis****– Update of serological criteria**

Variable	Cutoff	Points <sup>1</sup>
ANA or SMA/F-Actin	Positive <sup>2</sup>	1
ANA or SMA/F-Actin	Strongly positive <sup>3</sup>	
or LKM	≥1:40	2
or SLA	Positive	
IgG	>Upper normal limit	1
	>1.1 times upper normal limit	2
Liver histology (with evidence of hepatitis)	Compatible with AIH	1
	Typical AIH	2
Absence of viral hepatitis	Yes	2

≥6: probable AIH

≥7: definite AIH

<sup>1</sup>Addition of points achieved (maximum 2 points for autoantibodies);<sup>2</sup>IFT: ≥1:40 when assessed on tissue sections; ≥ 1:80 or 1:160 for ANA when assessed on HEp-2 cells, depending on local standards. ELISA with locally established cut-offs;<sup>3</sup>IFT: ≥1:80 when assessed on tissue sections; ≥ 1:160 or 1:320 for ANA when assessed on HEp-2 cells. ELISA with cut-offs established locally;

Note: if ELISA-based autoantibody assessment is negative despite high clinical suspicion of autoimmune hepatitis, IFT should be performed in addition.

36 552

37 553

38

39 554

41

42 555

43

44 556

45

46 557

47

48 558

49

50 559

51

52 560

53

54 561

55

56 562

57

58 563

59

60

61

62

63

64

65

564 **Figure legends**

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

565 **Figure 1. Flow-chart of patient cohorts included in this study.**

566  
567 **Figure 2. Receiver-operating-characteristic (ROC) curves showing the**  
568 **diagnostic value of ELISA for the diagnosis of AIH.** Diagnostic performance of (A)  
569 three different ANA ELISA and (B) a F-actin ELISA to discriminate between AIH and  
570 controls (distribution of diagnoses as shown in Figure 1). Area under the curve (AUC)  
571 values are indicated.


572  
573 **Figure 3. Receiver-operating-characteristic (ROC) curves showing the**  
574 **diagnostic performance of three different ANA ELISA in comparison with ANA**  
575 **immunofluorescence for the diagnosis of AIH.** Diagnostic performance is  
576 separately shown for cohorts from (A–B) Hamburg, (C–D) Larissa, and (E–F)  
577 Bologna. The distribution of diagnoses is shown in Figure 1. Area under the curve  
578 (AUC) values are indicated.

579  
580 **Figure 4. Receiver-operating-characteristic (ROC) curves showing the**  
581 **diagnostic performance of a F-actin ELISA in comparison with SMA**  
582 **immunofluorescence for the diagnosis of AIH.** Diagnostic performance is  
583 separately shown for cohorts from (A–B) Hamburg, (C–D) Larissa, and (E–F)  
584 Bologna. The distribution of diagnoses is shown in Figure 1. Area under the curve  
585 (AUC) values are indicated.


586  
587  
588  
589

590 **Figures**

591 **Figure 1:**

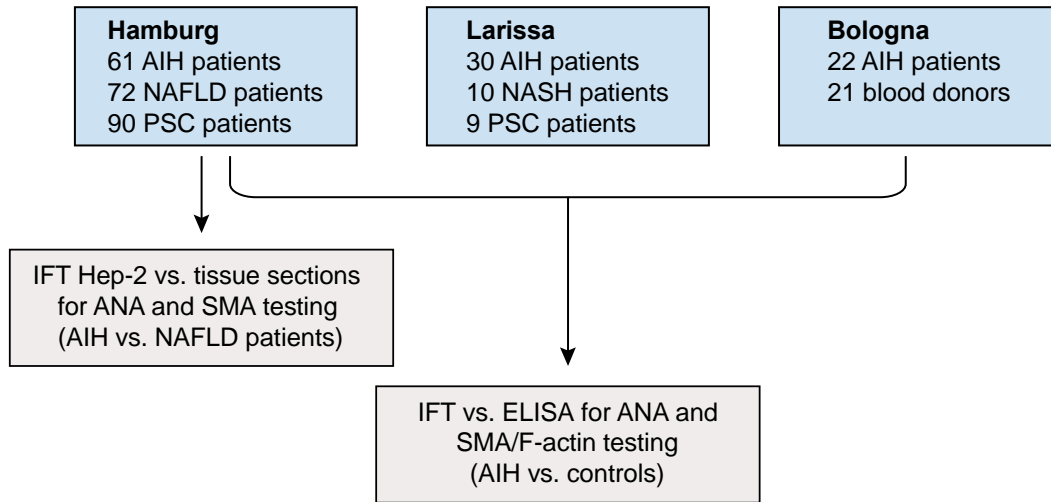


593 **Figure 2:**

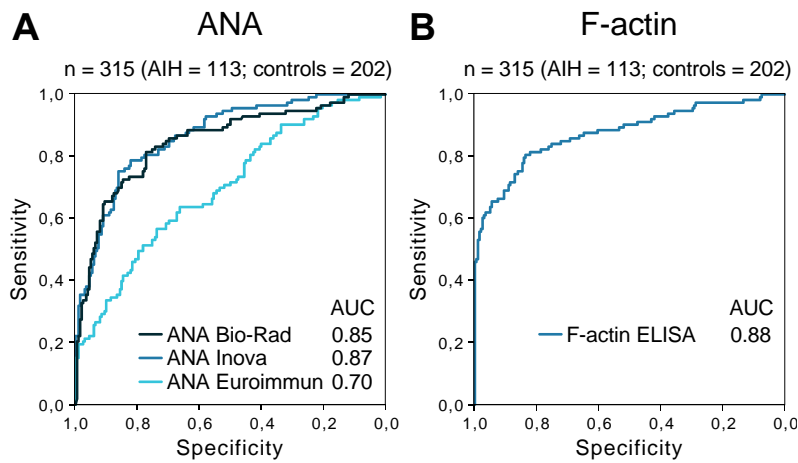

596  
597  
598  
599  
600  
601  
602  
603  
604  
605  
606  
607  
62  
63  
64  
65


608 **Figure 3:**

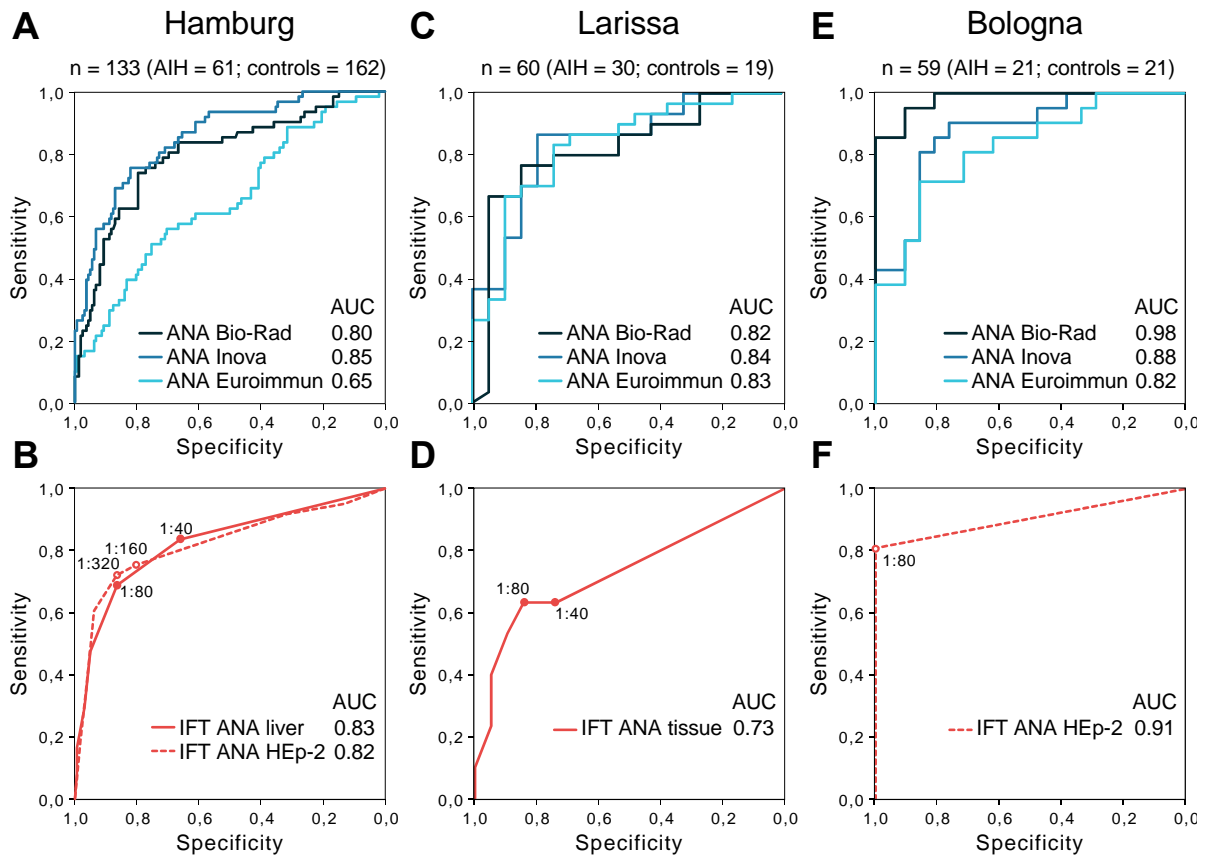

609

610

611 **Figure 4:**

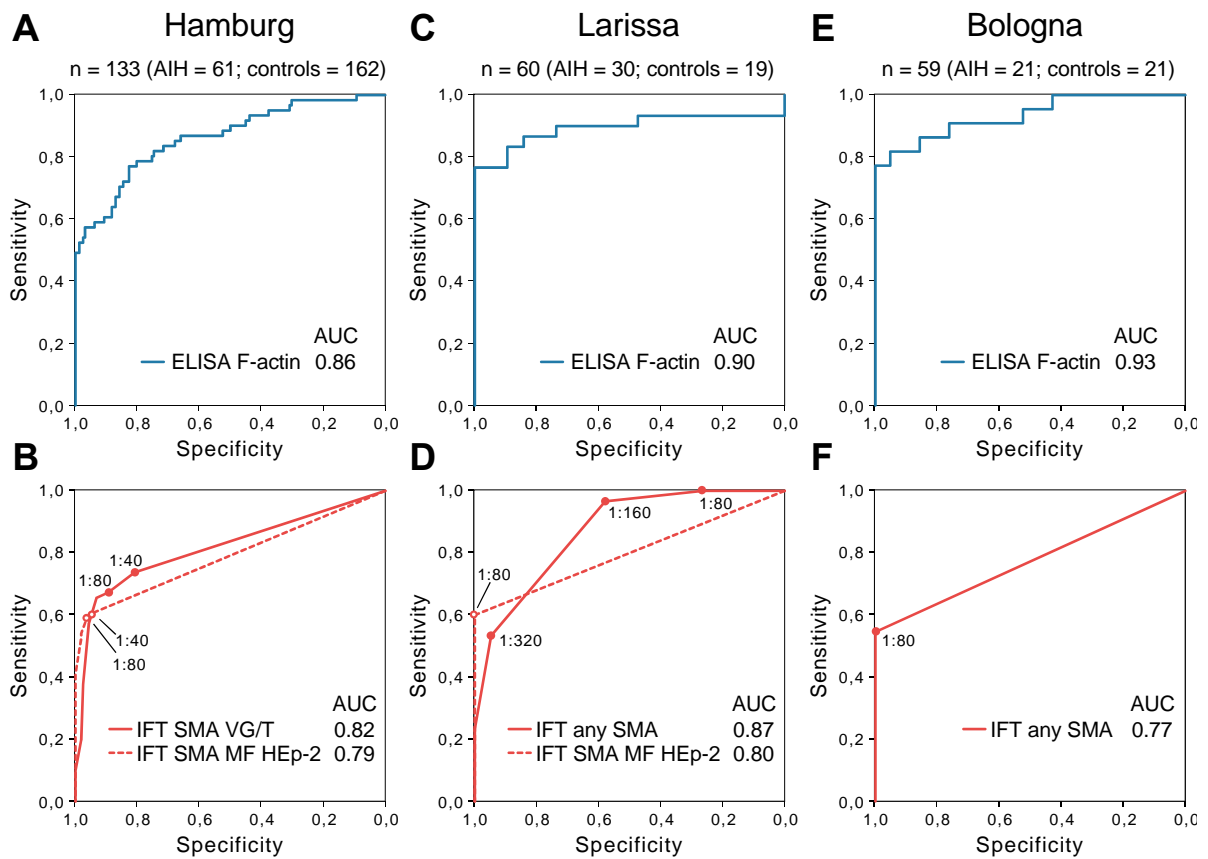

612

1  
2  
3  
4  
5  
6  
7  
8  
9  
10  
11  
12  
13  
14  
15  
16  
17  
18  
19  
20  
21  
22  
23  
24  
25  
26  
27  
28  
29  
30  
31  
32  
33  
34  
35  
36  
37  
38  
39  
40  
41  
42  
43  
44  
45  
46  
47  
48  
49  
50  
51  
52  
53  
54  
55  
56  
57  
58  
59  
60  
61  
62  
63  
64  
65

**Table 1. Sensitivity and specificity of ANA IFT for different tissue sections**

Substrate	Titer	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
HEp-2 cells	1:40	95.1	8.3	46.8	66.7	48.1
	1:80	91.8	36.1	54.9	83.9	61.7
	1:160	75.4	73.6	70.8	77.9	74.4
	1:320	72.1	76.4	72.1	76.4	74.4
	1:640	60.7	87.5	80.4	72.4	75.2
Primate liver	1:40	83.6	69.4	69.9	83.3	75.9
	1:80	68.9	80.6	75.0	75.3	75.2
	1:160	47.5	91.7	82.9	67.4	71.4
	1:320	47.5	91.7	82.9	67.4	71.4
	1:640	29.5	94.4	81.8	61.3	64.7
Rat kidney	1:40	75.4	73.6	70.8	77.9	74.4
	1:80	65.6	81.9	75.5	73.8	74.4
	1:160	52.5	87.5	78.1	68.5	71.4
	1:320	47.5	91.7	82.9	67.4	71.4
	1:640	34.4	93.1	80.8	62.6	66.2
Rat stomach	1:40	78.7	70.8	69.6	79.7	74.4
	1:80	67.2	81.9	75.9	74.7	75.2
	1:160	52.5	88.9	80.0	68.8	72.2
	1:320	44.3	91.7	81.8	66.0	69.9
	1:640	36.1	93.1	81.5	63.2	66.9
Any tissue positivity (primate liver, rat kidney, rat stomach)	1:40	85.3	65.3	67.5	83.9	74.4
	1:80	73.8	77.8	73.8	77.8	75.9
	1:160	52.5	87.5	78.1	68.5	71.4
	1:320	50.8	91.7	83.8	68.8	72.9
	1:640	37.7	93.1	82.1	63.8	67.7

AIH n=61; NAFLD n=72; ANA, antinuclear antibodies; HEp-2 cells, human epithelioma-2 cells; IFT, immunofluorescence test; NPV, negative predictive value; PPV, positive predictive value.

**Table 2. Sensitivity and specificity of SMA IFT for different patterns**

Substrate	Titer	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
HEp-2 (microfilaments)	1:40	60.7	94.4	90.2	73.9	79.9
	1:80	59.0	98.6	97.3	74.0	80.5
	1:160	54.1	98.6	97.1	71.7	78.2
	1:320	52.5	98.6	97.0	71.0	77.4
	1:640	41.0	100	100	66.7	72.9
Kidney SMA-V (vessels)	1:40	78.7	45.8	55.2	71.7	60.9
	1:80	73.8	72.2	69.2	76.5	72.9
	1:160	68.9	80.6	75.0	75.3	75.2
	1:320	62.3	88.9	82.6	73.6	76.7
	1:640	49.2	98.6	96.8	69.6	75.9
Kidney SMA-VG (vessels, glomeruli)	1:40	72.1	70.8	67.7	75.0	71.4
	1:80	65.6	88.9	83.3	75.3	78.2
	1:160	63.9	94.4	90.7	75.6	80.5
	1:320	55.7	97.2	94.4	72.2	78.2
	1:640	36.1	100	100	64.9	70.7
Kidney SMA-VGT (vessels, glomeruli tubuli)	1:40	52.5	93.1	86.5	69.8	74.4
	1:80	49.2	93.1	85.7	68.4	72.9
	1:160	44.3	95.8	90.0	67.0	72.2
	1:320	31.2	97.2	90.5	62.5	66.9
	1:640	23.0	100	100	60.5	64.7
Kidney SMA-VG or HEp2 microfilaments	1:40	75.4	69.4	67.7	76.9	72.2
	1:80	68.9	88.9	84.0	77.1	79.7
	1:160	65.6	94.4	90.9	76.4	81.2
	1:320	62.3	97.2	95.0	75.3	81.2
	1:640	44.3	100	100	67.9	74.4
Liver (bile canaliculi)	1:40	59.0	83.3	75.0	70.6	72.2
	1:80	49.2	95.8	90.9	69.0	74.4
	1:160	42.6	98.6	96.3	67.0	72.9
	1:320	39.3	98.6	96.0	65.7	71.4
	1:640	26.2	100	100	61.5	66.2
Stomach (tunica muscularis, lamina muscularis mucosa, interglandular fibrils)	1:40	83.6	45.8	56.7	76.7	63.2
	1:80	75.4	72.2	69.7	77.6	73.7
	1:160	72.1	80.6	75.9	77.3	76.7
	1:320	68.9	90.3	85.7	77.4	80.5
	1:640	54.1	97.2	94.3	71.4	77.4
Any SMA positivity	1:40	86.9	37.5	54.1	77.1	60.2
	1:80	80.3	69.4	69.0	80.7	74.4
	1:160	72.1	79.2	74.6	77.0	75.9
	1:320	72.1	88.9	84.6	79.0	81.2
	1:640	60.7	97.2	94.9	74.5	80.5

AIH n=61; NAFLD n=72; HEp-2 cells, human epithelioma-2 cells; IFT, immunofluorescence test; NPV, negative predictive value; PPV, positive predictive value; SMA, smooth muscle antibodies; VGT, vessel, glomeruli, tubuli.

**Table 3. Diagnostic value of ANA and F-Actin ELISA at cut-offs recommended by manufacturers**

ELISA	Assay	Cutoff	Sensitivity (%)	Specificity (%)	PPV (%)	NPV (%)	Accuracy (%)
ANA ELISA	Bio-Rad	≥ 1.0	65.5	88.6	76.3	82.1	80.3
		≥ 20	79.6	78.2	67.2	87.3	78.7
	Euroimmun	≥ 30	69.0	86.6	74.3	83.3	80.3
		≥ 1.0	22.1	95.0	71.4	68.6	68.9
F-Actin ELISA	Inova	≥ 20	81.4	82.2	71.9	88.8	81.9
		≥ 30	66.4	92.6	83.3	83.1	83.2

AIH n=113; controls n=202; distribution of diagnoses as shown in Figure 1; ANA, antinuclear antibodies; NPV, negative predictive value; PPV, positive predictive value.

**Table 4. Simplified criteria for autoimmune hepatitis****– Update of serological criteria**

Variable	Cutoff	Points <sup>1</sup>
ANA or SMA/F-Actin	Positive <sup>2</sup>	1
ANA or SMA/F-Actin or LKM or SLA	Strongly positive <sup>3</sup> ≥1:40 Positive	2
IgG	>Upper normal limit	1
	>1.1 times upper normal limit	2
Liver histology (with evidence of hepatitis)	Compatible with AIH	1
	Typical AIH	2
Absence of viral hepatitis	Yes	2

≥6: probable AIH

≥7: definite AIH

<sup>1</sup>Addition of points achieved (maximum 2 points for autoantibodies);<sup>2</sup>IFT: ≥1:40 when assessed on tissue sections; ≥ 1:80 or 1:160 for ANA when assessed on HEp-2 cells, depending on local standards. ELISA with locally established cut-offs;<sup>3</sup>IFT: ≥1:80 when assessed on tissue sections; ≥ 1:160 or 1:320 for ANA when assessed on HEp-2 cells. ELISA with cut-offs established locally;

Note: if ELISA-based autoantibody assessment is negative despite high clinical suspicion of autoimmune hepatitis, IFT should be performed in addition.



Figure 1

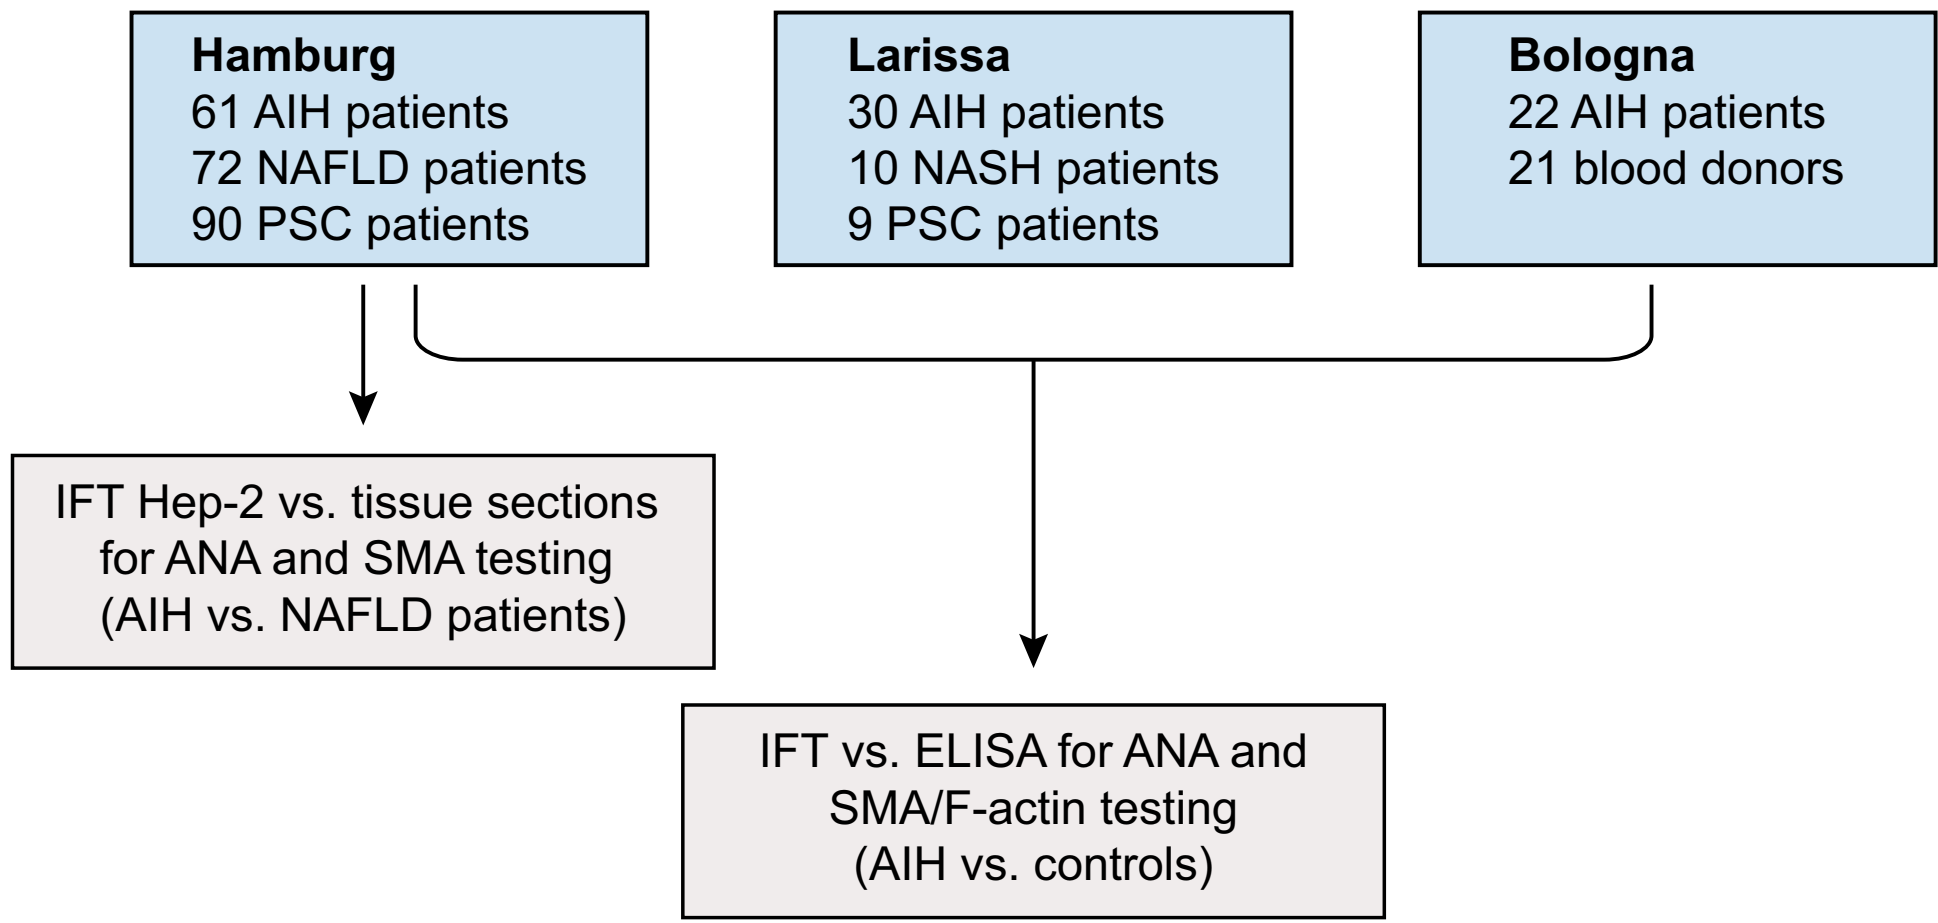


Figure 2

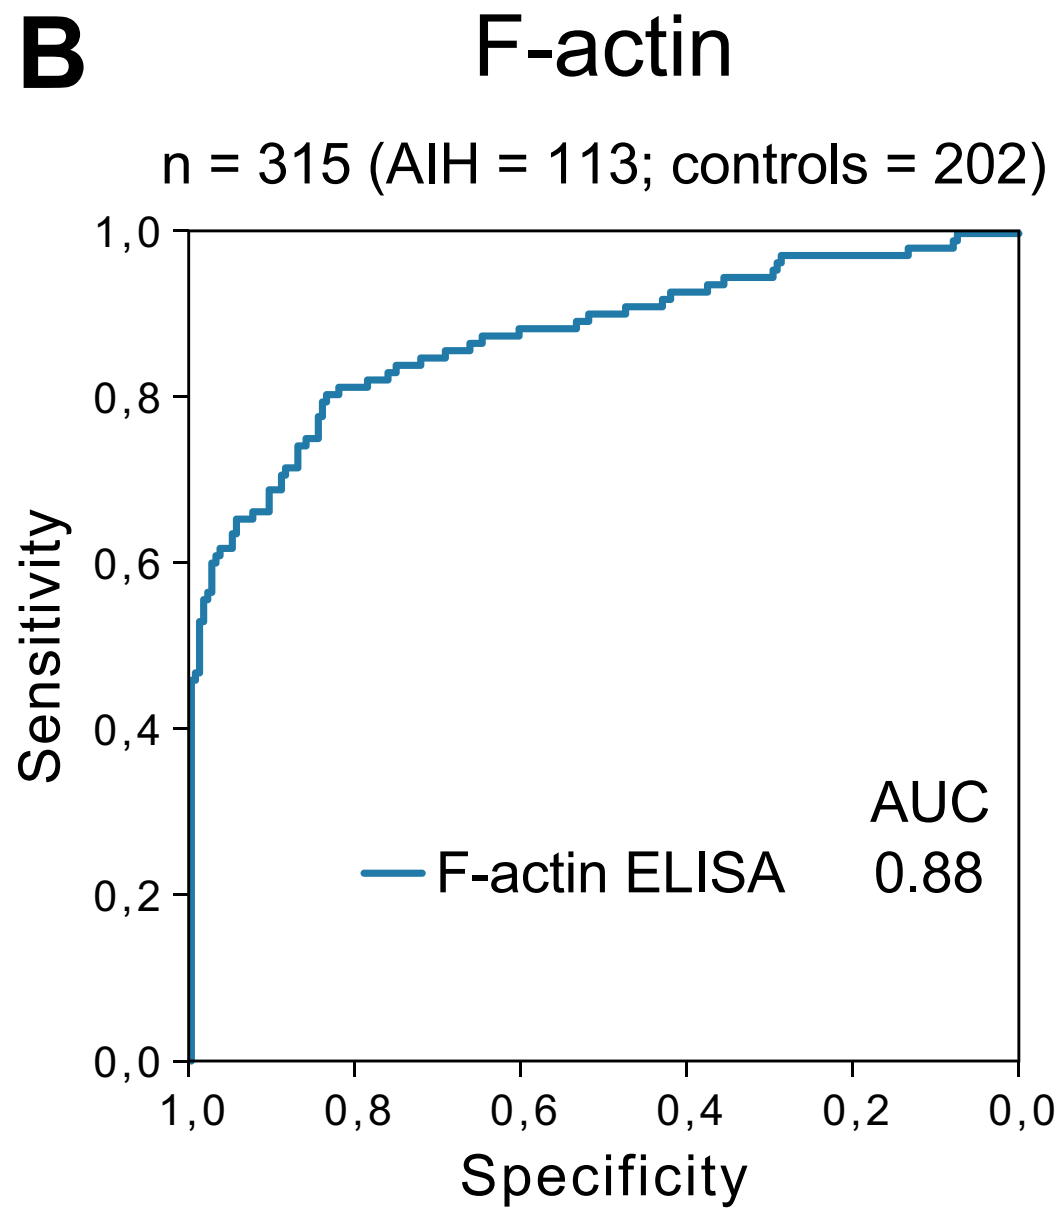
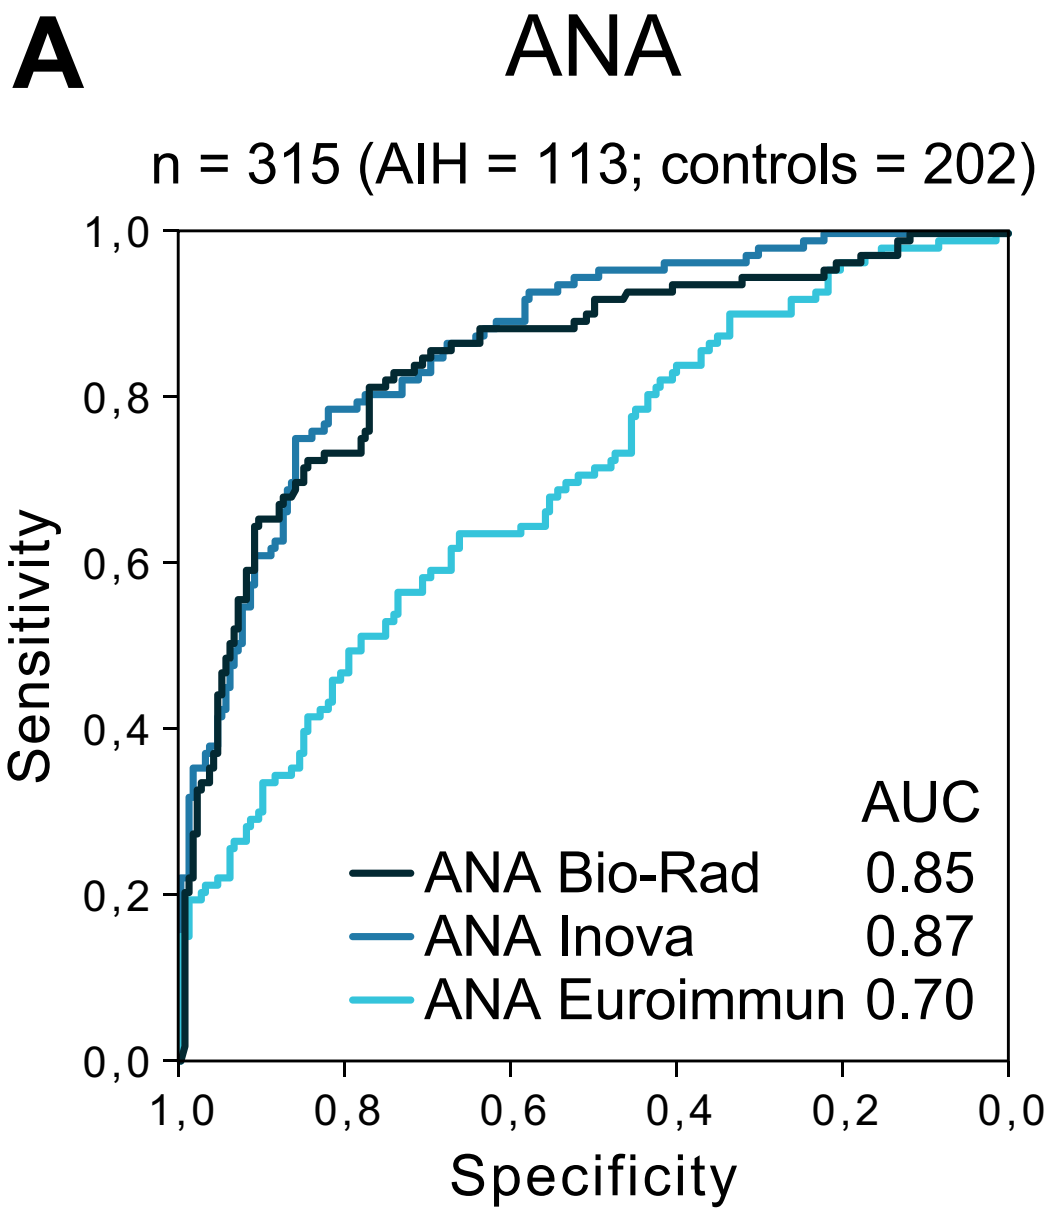


Figure 3














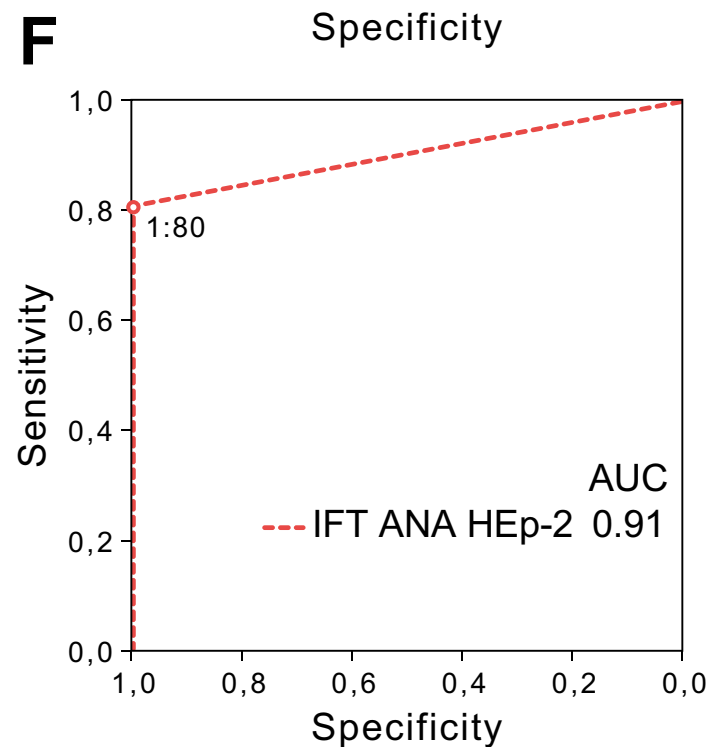


Figure 4

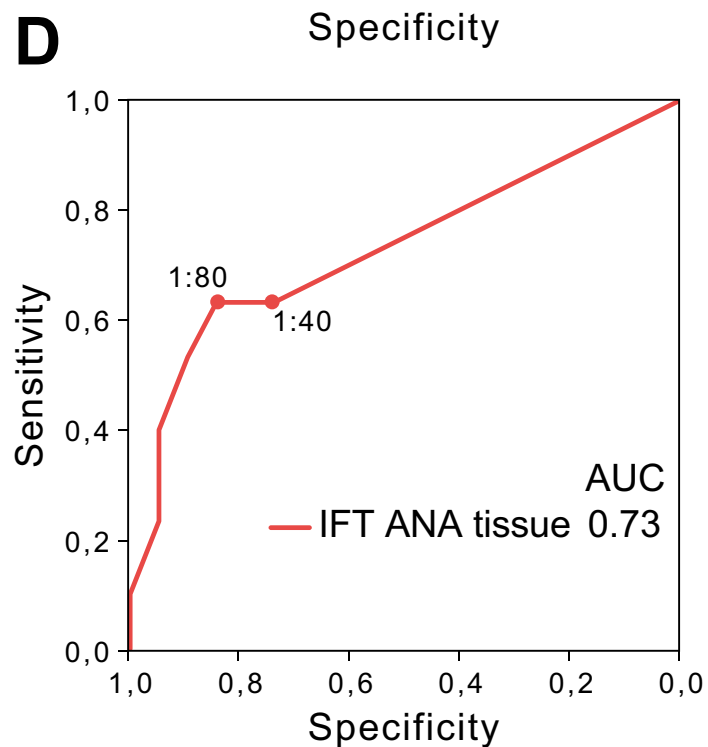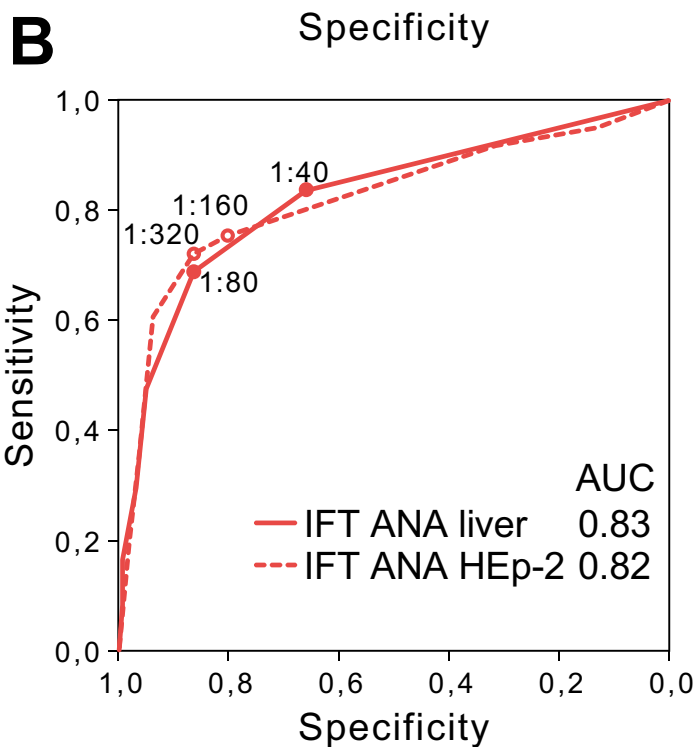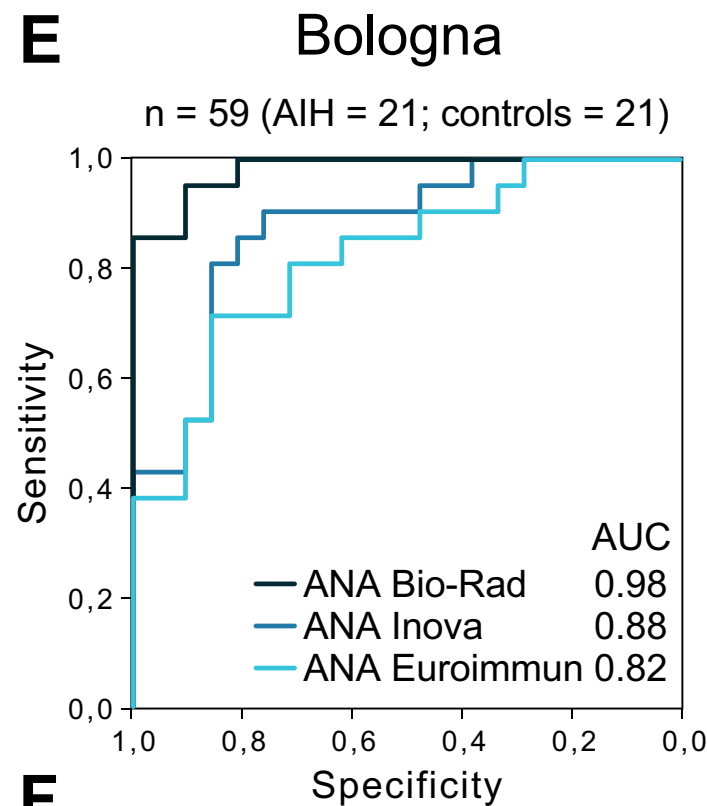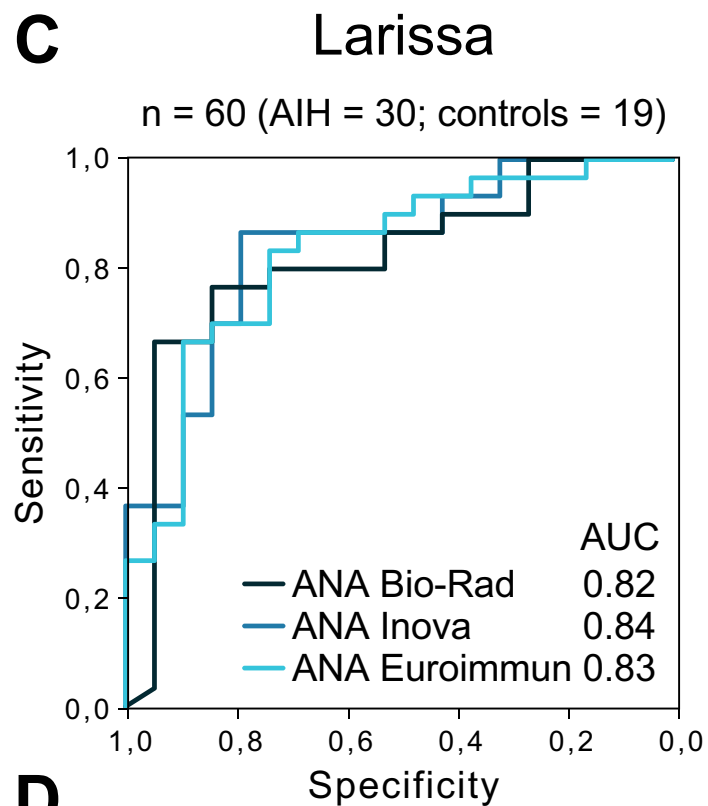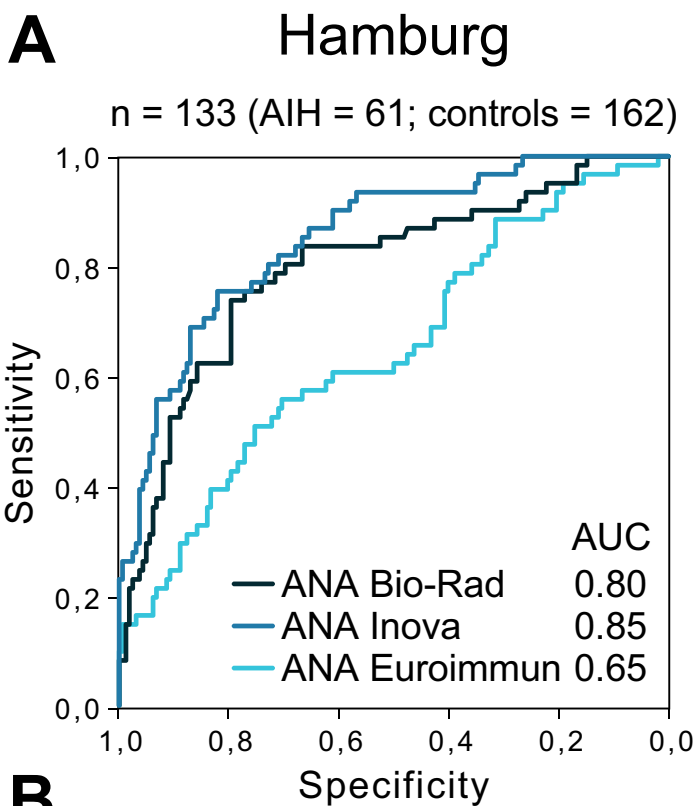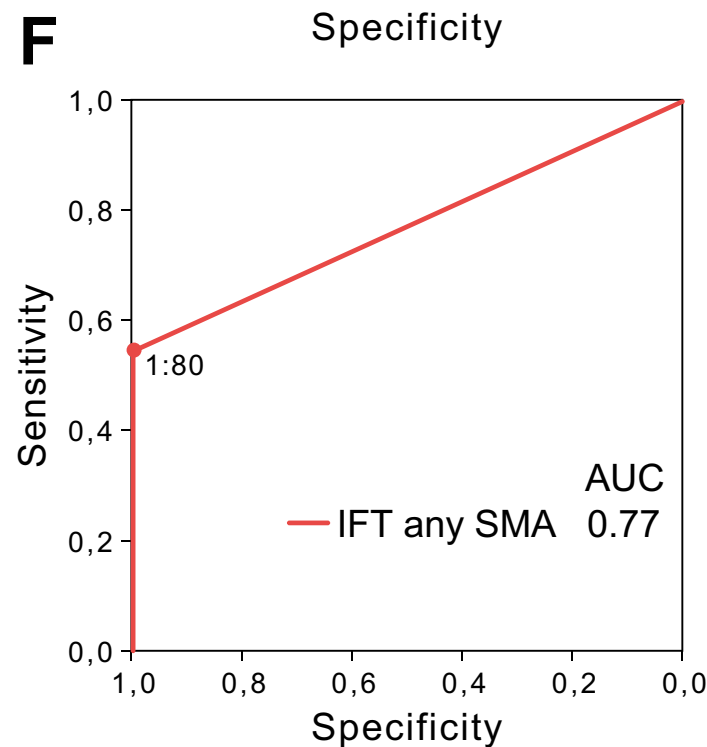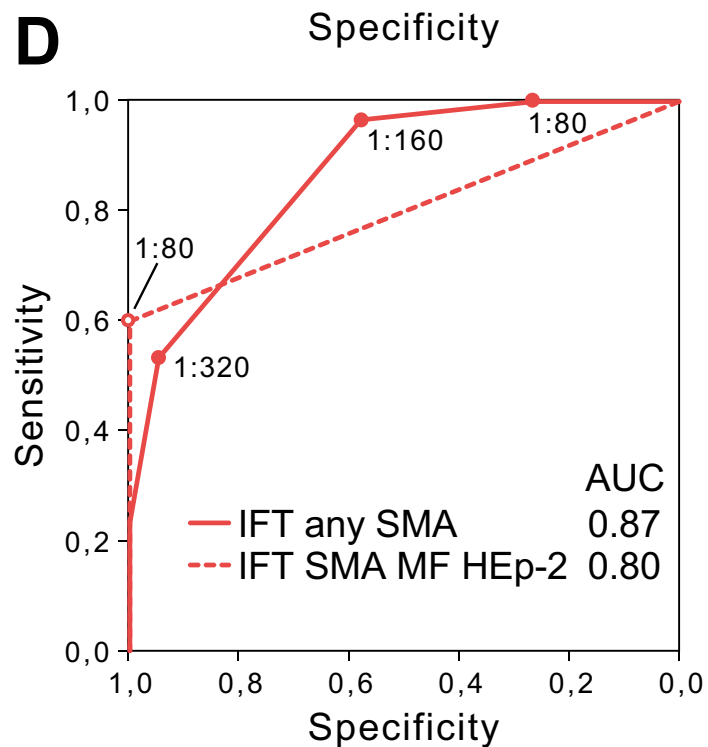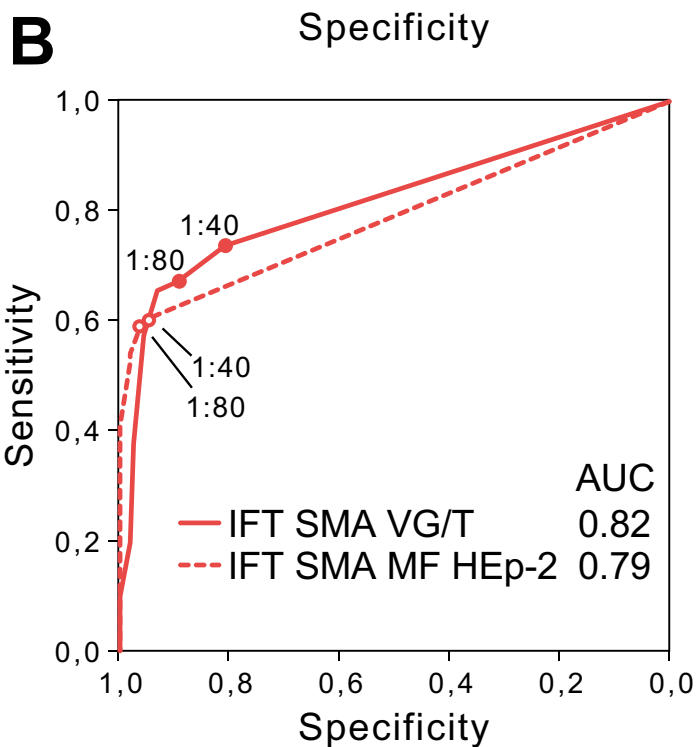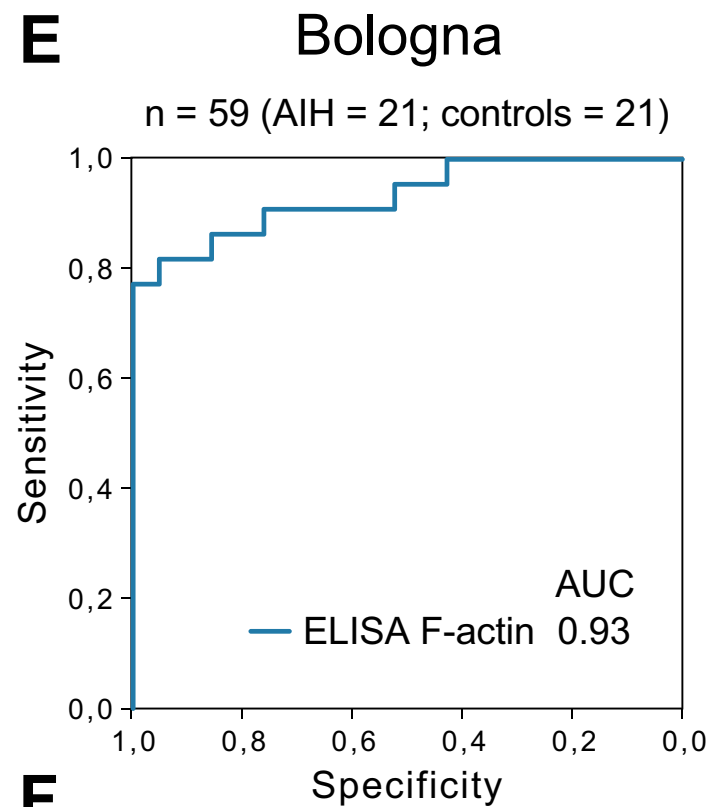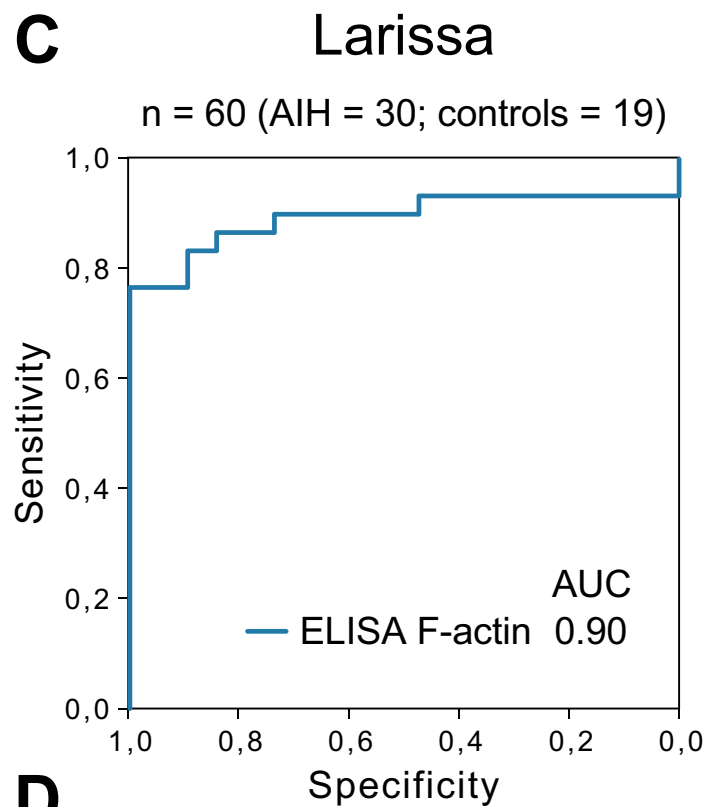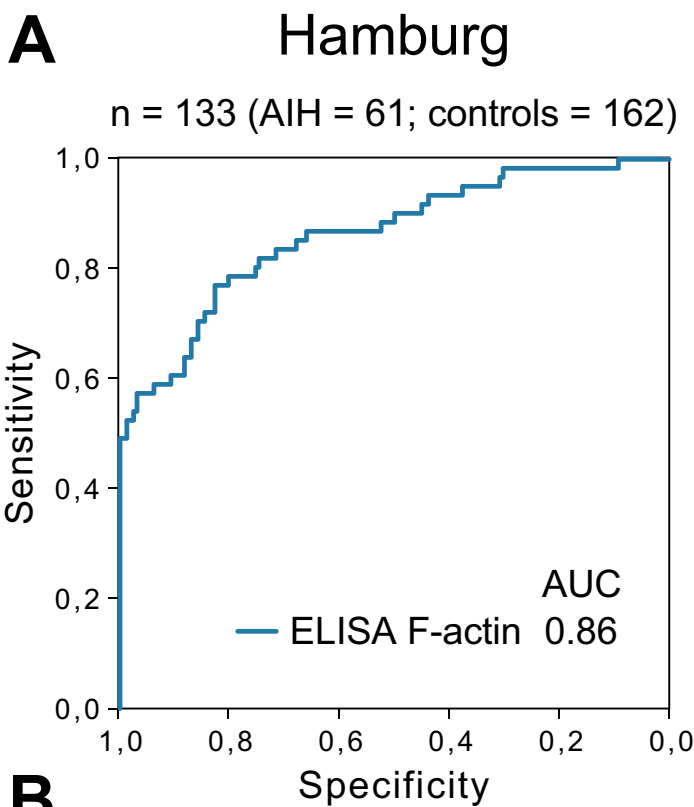

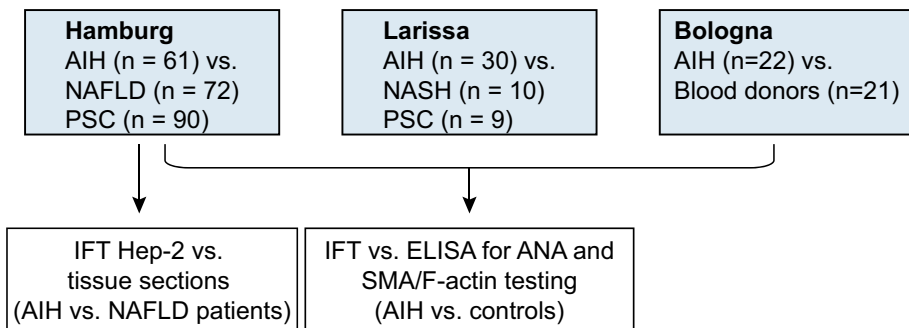

**Diagnostic performance of ANA and F-actin ELISA for the diagnosis of AIH**

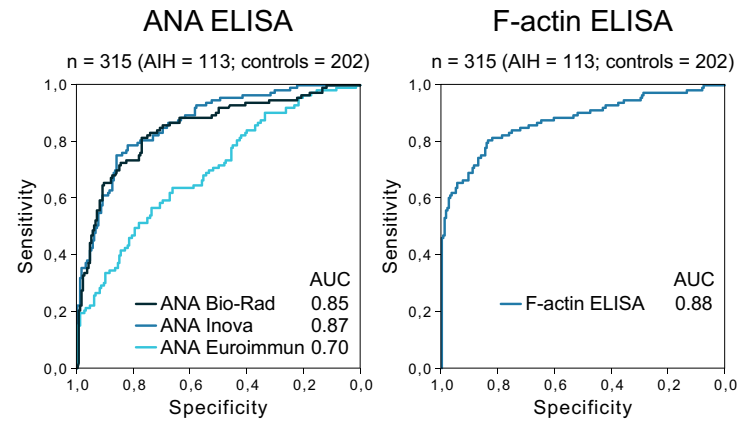

**The simplified criteria for the diagnosis of AIH – update of serological criteria**

Variable	Cutoff	Points
ANA or SMA/F-Actin	Positive <sup>1</sup>	1
ANA or SMA/F-Actin or LKM or SLA	Strongly positive <sup>2</sup> ≥1:40 Positive	2
IgG	>Upper normal limit	1
	>1.1 times upper normal limit	2
Liver histology (with evidence of hepatitis)	Compatible with AIH	1
	Typical AIH	2
Absence of viral hepatitis	Yes	2

≥6: probable AIH  
 ≥7: definite AIH

<sup>1</sup>IFT: ≥1:40 when assessed on tissue sections; ≥ 1:80 or 1:160 for ANA when assessed on HEp-2 cells, depending on local standards. ELISA with cut-offs validated locally;  
<sup>2</sup>IFT: ≥1:80 when assessed on tissue sections; ≥ 1:160 or 1:320 for ANA when assessed on HEp-2 cells. ELISA with cut-offs validated locally;  
 Note: if ELISA-based autoantibody assessment is negative despite of a high clinical suspicion for autoimmune hepatitis, IFT should be performed.

## Highlights

- IFT on HEp-2 cells is a valid alternative to the standard ANA assessment on rodent tissue sections in AIH when cutoffs titers are increased
- ANA ELISA and F-actin ELISA represent potential alternatives to IFT in the diagnosis of AIH
- ANA ELISA kits should include HEp-2 nuclear extracts to account for unrecognized autoantigens
- ELISA cutoffs need to be validated locally to be predictive in diagnosing AIH